







SURTEX INSTRUMENTS

Crafted to Excellence

• INTRODUCTION TO THE CATALOGUE

Thank you for your interest in Surtex sterilisation instruments and Surticon™ Sterile Container System. We remain committed to providing the highest quality products and customer service.

In this special catalogue you will find a comprehensive range of sterilisation instruments & Surticon Sterile Container System, which have been developed following detailed consultation with leading CSSD experts. Surtex instruments highly recommend use of these sterilisation instruments & Surticon Sterile Container System to achieve optimal sterilisation results for all your surgical instruments.

We appreciate your patronage and look forward to a successful relationship with you.

• ABOUT SURTEX INSTRUMENTS

Surtex Instruments is a privately owned medical technology company dedicated to innovation and excellence in crafting of surgical instruments. The company started as a specialist in reconstructive surgery instruments and based on its success and innovative drive gradually expanded to cover a vast range of surgical instruments.

We now manufacture over 8,000 surgical instruments and offer innovative solutions in trauma, gynecology, cardiovascular, microsurgery and dental surgery. All our products are available to view online where you can download our entire range of catalogues or request a printed version.

WHY IS SURTEX FOCUSED ON INSTRUMENTS QUALITY?

Surgeons are highly talented and skilled individuals. They operate under significant time constraints and are required to make split second decisions while performing complex operations. At Surtex we understand that in such a scenario the surgeon requires tools that are not just fit for the purpose but are reliable, dependable and crafted by a company that has a track record for relentless pursuit for excellence in the making of surgical instruments.

• AFFORDABLE QUALITY

Surgical instruments represent a significant proportion of hospital's total assets. Hospitals and health centers are often required to minimize costs of surgical instruments without impacting quality or patient's health. Decision makers tend to respond via group purchasing contracts & multiple quotes to shop around for the lowest price. However this approach has significant drawbacks as numerous instrument companies have focused towards competing on price alone with a disregard towards instruments quality while claiming their instruments to be guaranteed and free of defect.

The outcome for the buyer being a perceived notion of a quality instrument, which is actually little more than a knock-off and delivers only poor value for money.

At **Surtex Instruments** our success has been based on helping customers navigate successfully through the instrument procurement process by identifying real value for money through fair comparison. We believe that quality should be affordable and you should not pay too much for over priced brands and neither should you pay too much for a low quality instrument.

• SURTEX QUALITY STANDARDS

In European Union medical devices are subject to a series of uniform laws and the EC directive places rigid demands on surgical instruments. Surtex Instruments is proud to claim that we have always surpassed the legal requirements to ensure that each instrument reaching the surgeons hand is indeed a testament to surgical craftsmanship.

We are **BS EN ISO 13485:2012/ISO 9001:2008 (SGS UK)** certified and **CE** approved to ensure compliance with the standards defined in line with medical devices directive **93/42/EEC**.



• LIFE TIME WARRANTY

We encourage our customers to calculate lifetime costs prior to making purchase decisions and investing in surgical instruments.

Surtex Instruments are guaranteed for life* against manufacturing defects of material and workmanship. This means we will repair or replace free of charge any surgical instrument that does not meet its functional requirements when used for its intended purpose and maintained properly.



A member of the ABHI
ABHI
Health Tech For Life
Association of British HealthTech Industries

*Conditions apply.

OUR PRODUCT BRANDS



A new dimension in cutting and dissecting performance. Our class leading integral self-sharpening technology standard on all Surtex scissors enabling precise cutting with minimum force even after pro-longed use.



These Surtex premium scissors feature finely ground micro serrations along one blade of the scissor preventing tissue slippage. The ultra sharp edge of the other blade cuts through the tissue precisely and atraumatically.



Instruments with this symbol benefit from tungsten carbide (TC) inserts expertly bonded on the cutting edge of the instrument. This material is harder than stainless steel and enables the instruments to last up to 6 times longer than standard instruments.



A true craftsmanship masterpiece and surgeons favourite. These are the best scissors in our range and combine the features of SuperEdge™ & UltraCut™ into a perfect pair of scissors that is precise, durable and reliable.



The only choice when the perfect grip matters. Utilising Creep Feed technology individual teeth are grinded into hard wear resistant tungsten carbide (TC). The result is super sharp teeth with well-defined point and inserts with impeccable gripping properties and instruments that last up to 6 times longer.



These instruments have jaws, which are coated with diamond dust resulting in improved gripping enabling superior manipulation of sutures, needles and tissues.



Our specially designed high strength fibre grip handles resulting in lightweight instruments. These ergonomic handles provide the surgeon with excellent feel, better grip, reduced shock, and less hand fatigue.



Surtex ENT diagnostic and anaesthesia instruments featuring direct bulb illumination of xenon grade bulbs.



This range features distal fibre optic to carry light from xenon bulb allowing cold illumination on operating site in our ENT diagnostics and anaesthesia instruments.



Premium grade ENT diagnostics and anaesthesia instruments combining features of distal fibre optic technology and ultra bright LED illumination ensuring the best in clear vision of operating site.

CURRENT REFERENCE STANDARDS FOR SURTEx PRODUCTS

STANDARDS	CONTENTS OF THE STANDARD
BS EN ISO 9001:2008	Quality Management Systems certification standard.
BS EN ISO 13485:2003	Medical Devices – Quality Management Systems certification standard.
MDD 93/42/EEC, Annex II, Section 3.2	Medical Device Directive, 'EC Declaration of Conformity' (full quality assurance system).
MDD 93/42/EEC, Annex I	Essential Requirements for Medical Devices.
BS EN ISO 7153-1:2001 (BS 5194:Part 1:1991)	Surgical Instruments – Metallic materials part 1 - Stainless Steel
BS 5194:Part 2:1989	Specification for instruments with pivot joints (excluding cutting instruments)
BS 5194:Part 3:1985	Specification for Dissecting Forceps
BS 5194:Part 4:1985	Specification for scissors, shears, and other jointed cutting instruments
ISO 7151:1988	Surgical instruments – non-cutting, articulated instruments – general requirements & test methods
ISO 7740:2004	Scalpels with detachable blades - Fitting dimensions
ISO 7741:1986	Scissors and shears - General requirements and test methods
ISO 6508-1:2005 (DIN 50103-3:1995)	Specifies the method for Rockwell and Rockwell superficial hardness tests for metallic materials.
BS EN ISO 14971:2012	Medical Devices – Application of risk management to medical devices.
DIN 58298:2010-09	Medical instruments - Materials, finish and testing.
DIN 58299:1964-01	Serrations for surgical instruments; profile angles, groove distances.
DIN 58300:1982-02	Joints for surgical instruments.
HTM 2010	Recommendations for sterilization
AS/NZ 4187-2003	Cleaning, disinfecting & sterilising of re-usable surgical instruments

This information is available on the internet at
www.surtex-instruments.com

INSTRUCTIONS FOR REPROCESSING OF REUSABLE SURGICAL INSTRUMENTS

The following instructions are for all reusable medical devices supplied by Surtex Instruments Ltd, unless stated otherwise with the packaging of the product. These instructions are intended for use only by persons with the required specialist knowledge and training.

Warnings

- Follow instructions and warnings as issued by the manufacturers of any decontaminants, disinfectants and cleaning agents. Wherever possible avoid use of mineral acids and harsh, abrasive agents.
- No part of the process shall exceed 140 °C.
- Some sensitive materials (e.g. Aluminium) are damaged by high alkaline solutions (pH>10).
- Devices with long, narrow cannula, hinges and blind holes require particular attention during cleaning.

Note: When reprocessing medical devices, always handle with care, wearing protective clothing, gloves and eye-wear in accordance with local health & safety procedures.

Limitations on Reprocessing

- Repeated processing has minimal effect on these instruments.
- End of life normally determined by wear and damage in use.
- Any specific limitations on the number of reprocessing cycles shall be made available with instrument.

From Point of Use

Whenever possible, do not allow blood, debris or bodily fluids to dry on instruments. For best results and to prolong the life of the medical device reprocess immediately after use. If they cannot be reprocessed immediately, use an enzymatic foam spray cleaner to help prevent soil from drying.

Preparation for Decontamination

- Process all the instruments as soon as it is reasonably practical following use.
- Disassemble only where intended, without the use of tools unless specifically provided by the manufacturer. Instructions for dis assembly are available with the device, where required.

Cleaning: Automated

- Use only either CE marked or validated washer-disinfector machines and low foaming, non-ionizing cleaning agents and detergents following the manufacturer's instructions for use, warnings, concentrations and recommended cycles.
- Load instruments carefully, with any box joints and hinges open and so that any fenestration in instruments can drain.
- Place heavy instruments with care in the bottom of containers, taking care not to overload wash baskets.
- Place instruments with concave surfaces facing down to prevent pooling of water.
- Where possible, use appropriate attachments to flush inside reamers and devices with lumens or cannula.
- Ensure that soft, high purity water which is controlled for bacterial endo-toxins is used in the final rinse stage.

Note: Automated cleaning may not be suitable for all lumens and cannula in which case clean manually with a water jet gun, if available, and an appropriate brush (and stilette if provided) that reaches the depth of the feature. After manually cleaning, pass all devices through an automatic cleaning cycle to achieve disinfection.

Note: These instruments have been validated using a washer-disinfector cycle validated to include two cold rinses at <35 °C, a detergent cycle and a rinse cycle both at >50°C, a disinfection cycle operating at a temperature of between 80 °C and 90 °C for a minimum holding time of 1 minute (actual holding time in excess of 2 minutes 50 seconds) and a 20 minute drying cycle. The detergent used was low foaming, non-ionizing spray wash detergent cleaner (max 12pH) and the rinse aid a neutral pH low foaming, non-ionic surfactant with isopropyl alcohol.

Cleaning: Manual

- Manual cleaning is not advised if an automatic washer-disinfector is available. If the equipment is not available, use the following process:-
- Use a double sink system (wash/rinse) dedicated for instrument cleaning (not used for hand washing). Ensure that the water temperature does not exceed 35 of the re-processor to ensure that the reprocessing as actually performed using equipment, materials and personnel in the reprocessing facility achieve the desired result. This requires validation and routine monitoring of the process. Likewise any deviation by the re-processor from the instructions provided must be properly evaluated for effectiveness and potential adverse consequences.
 - In the first sink, keeping the instrument submerged, with an autoclavable brush, apply CE marked cleaning solution to all surfaces until all soil has been removed. Pay particular attention to serrations, teeth, ratchets and hinges, always brushing away from the body and avoiding splashing. Ensure rongeurs and hinged instruments are thoroughly cleaned in both open and closed positions.
 - In the second sink, rinse instruments thoroughly with soft, high purity water which is controlled for bacterial endotoxins, so that the water reaches all parts of the instrument, then carefully hand dry or use a drying cabinet.

Note: Manual Cleaning is NOT a disinfection process: When manual cleaning is used it may not be possible to disinfect the device prior to further handling.

Cleaning Inspection

- After cleaning visually inspect, visually inspect all surfaces, cannulations, ratchets, joints, holes and lumens for complete removal of soil and fluids. If ANY soil or fluid is still visible, return the instrument for repeat decontamination.

Maintenance

- Apply surgical grade lubricant to hinges, joints and moving parts as per the lubricant manufacturer's instructions.

Continued on next page

Inspection and Functional Testing

- Visually inspect and check: - all instruments for damage and wear; cutting edges are free from nicks and present a continuous edge; jaws and teeth align correctly; all articulated instruments have a smooth movement without excess play; locking mechanisms (such as ratchets) fasten securely and close easily; long, slender instruments are not distorted; any component parts fit and assemble correctly with mating components.
- Remove for repair and replacement any blunt, worn out, flaking, fractured or damaged instruments.

Note: If an instrument is returned to the manufacturer / supplier, the instrument must be decontaminated and sterilized and be accompanied with the relevant documented evidence.

Packaging

- All instruments to be packed following local protocol in accordance with ISO 11607-1 or AAMI/CSR technique.

Sterilization (USA)

- Autoclave should comply with the requirements of, and be validated and maintained in accordance with ANSI/AAMI ST79.
- Pre-Vacuum moist heat sterilization operating at temperature 132 °C bar for a minimum holding time of 4 minutes always following the instructions of the machine manufacturer.
- When sterilizing multiple instruments in one autoclave cycle, ensure that the sterilizer manufacturers stated maximum load is not exceeded.
- Ensure instruments are dry before sterilization.

Sterilization (Outside USA)

- Autoclave should comply with the requirements of, and be validated and maintained in accordance with EN 285, EN 13060, EN ISO 17665.
- Either CE marked or validated vacuum autoclave operating at 134-137 °C bar for a minimum holding time of 3 minutes always following the instructions of the machine manufacturer.
- When sterilizing multiple instruments in one autoclave cycle, ensure that the sterilizer manufacturers stated maximum load is not exceeded.

Storage

- Ensure instruments are dry before storage, and stored in dry, clean conditions at an ambient room temperature.

Additional Information

- Other forms of cleaning (i.e. ultrasonic) and sterilization (i.e. Low temperature steam and Formaldehyde, Ethylene Oxide and Gas Plasma) are available. However, always follow the instructions for use as issued by the manufacturer and always consult with them if in any doubt over the suitability of any process used.
- Cleaning and sterilizing guidelines are available in HTM 2030 and HTM 2010. Contact: The NHS Estates Stationers Office Publications Cent for details at www.tsonline.gov.uk. For further information contact: NHS Estates Information Center, Department of Health, 1 Trevelyan Square, Boar Lane, Leeds, LS1 6AE, UK or visit www.nhsestates.gov.uk.

Note: It is the responsibility of the re-processor to ensure that the reprocessing as actually performed using equipment, materials and personnel in the reprocessing facility achieve the desired result. This requires validation and routine monitoring of the process. Likewise any deviation by the re-processor from the instructions provided must be properly evaluated for effectiveness and potential adverse consequences.


Surticon™ Sterile Container System

BioClean™

BioFree™



The locking mechanism of the lid can stand stationary in every position upto 180°.

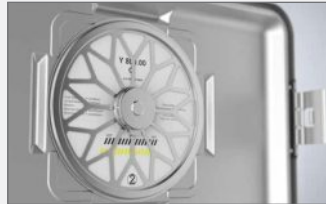

The silicone gaskets of the lids ensure security of the sterilization process.



Silicone handle are available in six different colors.



The security seals are removed only while opening the containers lids to prevent unauthorized use.




The colored identification labels of the containers are changeable.



The fixation clamps for holding the cylindrical instruments are available in different sizes.



The locking mechanism of the lid can be used as the lid handle.

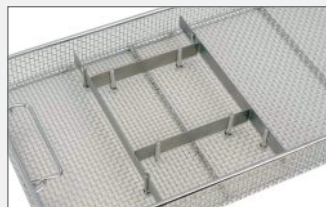

The plates and holding pins facilitate separation inside the wire mesh basket kits as desired.



The silicone mats, firmly hold micro instruments in their place.



The containers can be stacked on top of each other during storage. (See user manual).




Spiral holders, hold the instruments securely.



The locking latches of the filter holders facilitate quick change of filters.

SurticonTM Sterilization Container Production Process

Starting from production to distribution, SurticonTM Sterilization Container Systems are manufactured through several processes to provide durable and long-lasting products.

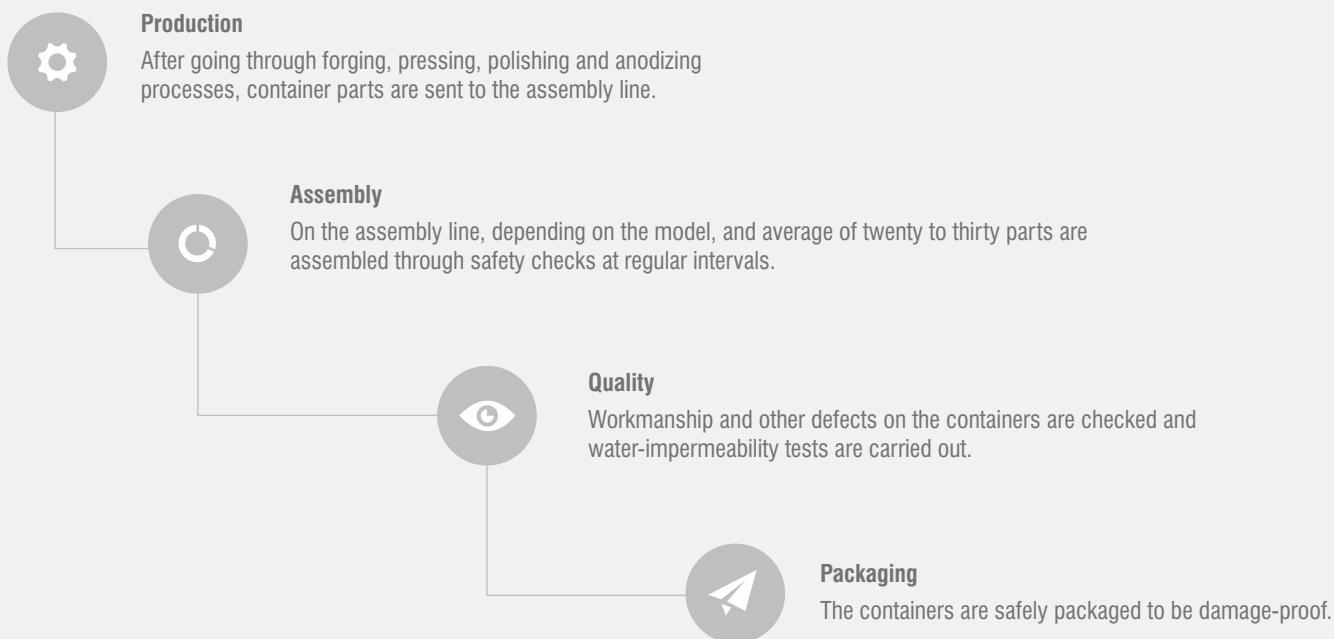


Assembly Components & Accessories

- | | | |
|----------------------------|---------------------------|--------------------------|
| 1. Container Base | 11. Indicator Spring | 21. Hinge Rod |
| 2. Notch Locking | 12. Identification Labels | 22. Silicone Gasket |
| 3. Silicone | 13. Indicator | 23. Filter Retainer Lock |
| 4. Front Plate | 14. Lid | 24. Filter Retainer |
| 5. Notch Spring | 15. Safety Lid | 25. Silicone Gasket |
| 6. Indicator & Label Sloth | 16. Screw | 26. Paper Filter |
| 7. Sloth Screw | 17. Centering Pin | 27. Security Seal |
| 8. Handle Shaft | 18. Riveting Pin | |
| 9. Handle Silicone | 19. Hinge Plate | |
| 10. Sloth Spring | 20. Locking Plate | |




BioFreeTM Sterilization Mechanism For Surticon BioFreeTM Sterile Container Systems

1




Before sterilization the valves are in relax position.

2

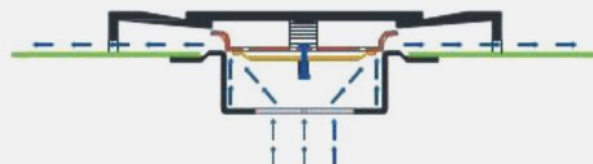


During sterilization the valves open completely by vacuum to evacuate dry air out of the container.

3

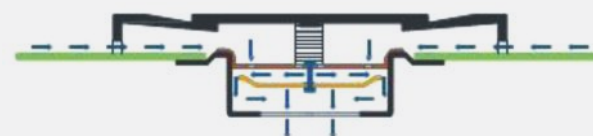


At the end of sterilization cycle the valves then open in reverse direction by vacuum and the sterilization cycle completes.

4

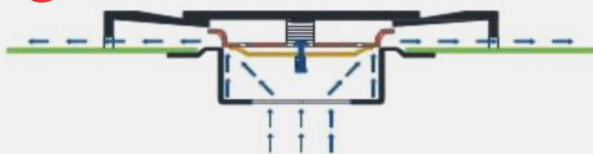

















At the end of sterilization cycle the sterilizer equates the pressure level and the valves of BioFreeTM model close down.

5



After sterilization the valves go back to relax position.

**Compliance scheme of Surticon Sterile Container System for steam sterilization procedures as per
DIN 58953, part 9 (in accordance with the May 1987 issue)**

Sterilization Container	Packing		Steam Sterilization Procedure According to DIN 58946 Part 1				
	Description	Symbolic Representation and Packing System	Gravitation Procedure	Pre-Vacuum Procedure	Fractional Vacuum Procedure	Fractional Flow Procedure	Steam Injection Procedure
With Filters (STB-F)	Textiles in sterilization container with filter in lid and bottom according to DIN 58952 part 1		+	+	+	+	+
			○	○	+	+	+
	Textiles in sterilization container with filter in lid and bottom not perforated according to DIN 58952 part 1		-	-	+	+	+
			-	-	+	+	○
	Textiles in sterilization container with filter in lid and bottom according to DIN 58952 part 1		○	+	+	+	+
			-	○	+	+	+
	Instruments in wire basket acc. To DIN 58952 part III in sterilization container with filter in lid and bottom acc. to DIN 58952 part 1		+ ³⁾	+	+	+	+
	Instruments in wire basket acc. To DIN 58952 part III in sterilization container with filter in lid and bottom not perforated acc. to DIN 58952 part 1		-	+ ²⁾	+ ²⁾	+ ²⁾	+ ²⁾
	Instruments in wire basket acc. To DIN 58952 part III, in sterilization container with filter in lid & bottom not perforated acc. to DIN 58952 part 1		○	+	+	+	+
			○	+	+	+	+
With Valves (STB-V)	Textiles in sterilization container with valves in lid and bottom acc. To DIN 58952 part 1		-	○	+	+	○
			-	-	+	+	○
	Textiles in sterilization container with valves in lid and bottom acc. To DIN 58952 part 1.		-	-	+	+	-
			-	-	+	+	-
	Instruments in wire basket in sterilization container with valve in lid and bottom		-	+ ²⁾	+ ²⁾	+ ²⁾	+ ²⁾
	Instruments in wire basket in sterilization container with valve in lid and not perforated		-	+ ²⁾	+ ²⁾	+ ²⁾	+ ²⁾

Explanation of Symbols: + Applicable - Not Applicable ○ Limited Application

1) In order to avoid mistakes with regards to service, operation and/or when loading the sterilizer, please refer to table 1 for correct or wrong combination of sterilization containers for standardized steam sterilization procedures.


2) Only sterilization containers guaranteeing evaporation or discharge of condensate are suitable above.

3) Gravitation procedures having no drying device do not guarantee a sufficient after-drying effect.

TABLE OF CONTENTS

■ Surticon TM 1/1 Sterile Container	1 - 6
Surticon TM 3/4 Sterile Container	10 - 15
Surticon TM 1/2 Sterile Container	18 - 23
Surticon TM Sterile Container Dental Model	27 - 28
Surticon TM Sterile Container Mini Model	32 - 33
Surticon TM Sterile Container Implant Model	36 - 37
Surticon TM Sterile Container Scopy Model	38 - 39
Surticon TM Sterilizing Cases and Accessories	40 - 43 ■

Surticon™ 1/1 BioClean™ Sterile Container
Perforated Lid



BioClean™



ORDERING INFORMATION:

585 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-300-01
	Yellow	ST-300-02
	Green	ST-300-03
	Blue	ST-300-04
	Red	ST-300-05
	Black	ST-300-06

585 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-302-01
	Yellow	ST-302-02
	Green	ST-302-03
	Blue	ST-302-04
	Red	ST-302-05
	Black	ST-302-06


585 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-304-01
	Yellow	ST-304-02
	Green	ST-304-03
	Blue	ST-304-04
	Red	ST-304-05
	Black	ST-304-06

585 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-306-01
	Yellow	ST-306-02
	Green	ST-306-03
	Blue	ST-306-04
	Red	ST-306-05
	Black	ST-306-06

585 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-308-01
	Yellow	ST-308-02
	Green	ST-308-03
	Blue	ST-308-04
	Red	ST-308-05
	Black	ST-308-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM 1/1 BioCleanTM Sterile Container
Perforated Lid & Bottom



BioCleanTM



ORDERING INFORMATION:

585 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-310-01
	Yellow	ST-310-02
	Green	ST-310-03
	Blue	ST-310-04
	Red	ST-310-05
	Black	ST-310-06

585 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-312-01
	Yellow	ST-312-02
	Green	ST-312-03
	Blue	ST-312-04
	Red	ST-312-05
	Black	ST-312-06

585 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-314-01
	Yellow	ST-314-02
	Green	ST-314-03
	Blue	ST-314-04
	Red	ST-314-05
	Black	ST-314-06

585 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-316-01
	Yellow	ST-316-02
	Green	ST-316-03
	Blue	ST-316-04
	Red	ST-316-05
	Black	ST-316-06

585 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-318-01
	Yellow	ST-318-02
	Green	ST-318-03
	Blue	ST-318-04
	Red	ST-318-05
	Black	ST-318-06

ST

SURTICONTM STERILE CONTAINER SYSTEM

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 1/1 BioClean™ Sterile Container (With Safety Lid) Perforated Lid



BioClean™



ORDERING INFORMATION:

585 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-320-01
	Yellow	ST-320-02
	Green	ST-320-03
	Blue	ST-320-04
	Red	ST-320-05
	Black	ST-320-06

585 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-322-01
	Yellow	ST-322-02
	Green	ST-322-03
	Blue	ST-322-04
	Red	ST-322-05
	Black	ST-322-06

585 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-324-01
	Yellow	ST-324-02
	Green	ST-324-03
	Blue	ST-324-04
	Red	ST-324-05
	Black	ST-324-06

585 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-326-01
	Yellow	ST-326-02
	Green	ST-326-03
	Blue	ST-326-04
	Red	ST-326-05
	Black	ST-326-06

585 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-328-01
	Yellow	ST-328-02
	Green	ST-328-03
	Blue	ST-328-04
	Red	ST-328-05
	Black	ST-328-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM 1/1 BioCleanTM Sterile Container (With Safety Lid)
Perforated Lid & Bottom



BioCleanTM



ST

SURTICONTM STERILE CONTAINER SYSTEM

ORDERING INFORMATION:

585 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-330-01
	Yellow	ST-330-02
	Green	ST-330-03
	Blue	ST-330-04
	Red	ST-330-05
	Black	ST-330-06

585 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-332-01
	Yellow	ST-332-02
	Green	ST-332-03
	Blue	ST-332-04
	Red	ST-332-05
	Black	ST-332-06


585 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-334-01
	Yellow	ST-334-02
	Green	ST-334-03
	Blue	ST-334-04
	Red	ST-334-05
	Black	ST-334-06

585 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-336-01
	Yellow	ST-336-02
	Green	ST-336-03
	Blue	ST-336-04
	Red	ST-336-05
	Black	ST-336-06

585 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-338-01
	Yellow	ST-338-02
	Green	ST-338-03
	Blue	ST-338-04
	Red	ST-338-05
	Black	ST-338-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM 1/1 BioFreeTM Sterile Container
Perforated Lid



BioFreeTM



ORDERING INFORMATION:

585 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-340-01
	Yellow	ST-340-02
	Green	ST-340-03
	Blue	ST-340-04
	Red	ST-340-05
	Black	ST-340-06

585 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-342-01
	Yellow	ST-342-02
	Green	ST-342-03
	Blue	ST-342-04
	Red	ST-342-05
	Black	ST-342-06

585 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-344-01
	Yellow	ST-344-02
	Green	ST-344-03
	Blue	ST-344-04
	Red	ST-344-05
	Black	ST-344-06

585 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-346-01
	Yellow	ST-346-02
	Green	ST-346-03
	Blue	ST-346-04
	Red	ST-346-05
	Black	ST-346-06

585 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-348-01
	Yellow	ST-348-02
	Green	ST-348-03
	Blue	ST-348-04
	Red	ST-348-05
	Black	ST-348-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM 1/1 BioFreeTM Sterile Container
Perforated Lid & Bottom



BioFreeTM



ST

SURTICONTM STERILE CONTAINER SYSTEM

ORDERING INFORMATION:

585 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-350-01
	Yellow	ST-350-02
	Green	ST-350-03
	Blue	ST-350-04
	Red	ST-350-05
	Black	ST-350-06

585 x 280 x 160 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-352-01
	Yellow	ST-352-02
	Green	ST-352-03
	Blue	ST-352-04
	Red	ST-312-05
	Black	ST-312-06


585 x 280 x 175 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-354-01
	Yellow	ST-354-02
	Green	ST-354-03
	Blue	ST-354-04
	Red	ST-354-05
	Black	ST-354-06

585 x 280 x 235 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-356-01
	Yellow	ST-356-02
	Green	ST-356-03
	Blue	ST-356-04
	Red	ST-356-05
	Black	ST-356-06

585 x 280 x 295 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-358-01
	Yellow	ST-358-02
	Green	ST-358-03
	Blue	ST-358-04
	Red	ST-358-05
	Black	ST-358-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ Sterile 1/1 Instrument Basket

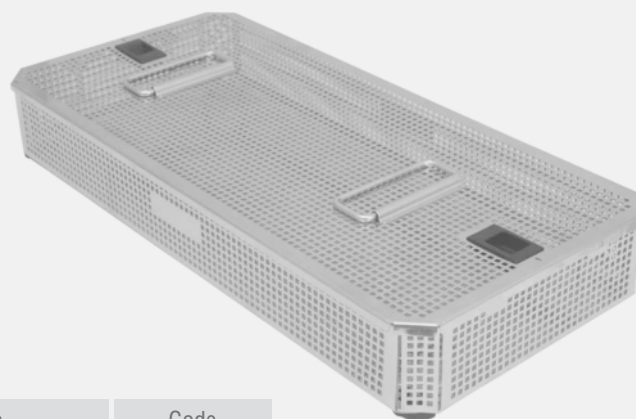

ORDERING INFORMATION:

Without Lid	Size	Code	With Lid	Size	Code
	484 x 252 x 25 mm	ST-380-01		488 x 256 x 25 mm	ST-382-01
	484 x 252 x 45 mm	ST-380-02		488 x 256 x 45 mm	ST-382-02
	484 x 252 x 65 mm	ST-380-03		488 x 256 x 65 mm	ST-382-03
	484 x 252 x 95 mm	ST-380-04		488 x 256 x 95 mm	ST-382-04
	539 x 252 x 25 mm	ST-380-05		543 x 256 x 25 mm	ST-382-05
	539 x 252 x 45 mm	ST-380-06		543 x 256 x 45 mm	ST-382-06
	539 x 252 x 65 mm	ST-380-07		543 x 256 x 65 mm	ST-382-07
	539 x 252 x 95 mm	ST-380-08		543 x 256 x 95 mm	ST-382-08

Surticon™ Sterile 1/1 Wire Mesh Basket



ORDERING INFORMATION:

Without Lid	Size	Code	With Lid	Size	Code
	480 x 250 x 30 mm	ST-384-01		480 x 250 x 30 mm	ST-386-01
	480 x 250 x 50 mm	ST-384-02		480 x 250 x 50 mm	ST-386-02
	480 x 250 x 70 mm	ST-384-03		480 x 250 x 70 mm	ST-386-03
	480 x 250 x 100 mm	ST-384-04		480 x 250 x 100 mm	ST-386-04
	540 x 250 x 30 mm	ST-384-05		540 x 250 x 30 mm	ST-386-05
	540 x 250 x 50 mm	ST-384-06		540 x 250 x 50 mm	ST-386-06
	540 x 250 x 70 mm	ST-384-07		540 x 250 x 70 mm	ST-386-07
	540 x 250 x 100 mm	ST-384-08		540 x 250 x 100 mm	ST-386-08


Sterile Container System
 Sterilcontainer System
 Sistema de recipiente estéril
 Système de récipient stérile
 Sterili Container System

ST
SURTICON™ STERILE CONTAINER SYSTEM

Surticon™ Sterile 1/1 Divider

ORDERING INFORMATION:


2 Partitions	Size	Code
	540 x 250 x 130 mm	ST-390-01
	540 x 250 x 180 mm	ST-390-02
3 Partitions	Size	Code
	540 x 250 x 130 mm	ST-392-01
	540 x 250 x 180 mm	ST-392-02

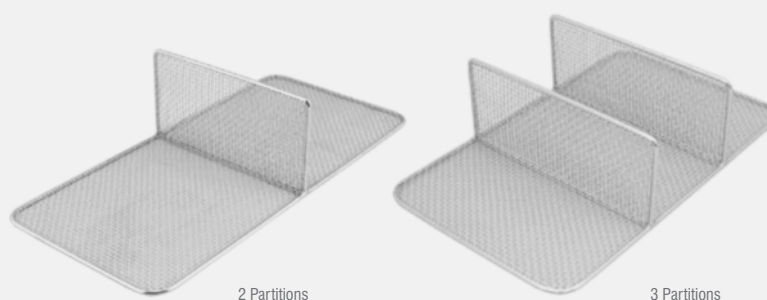

Surticon™ Sterile 1/1 Drape Retainer

ORDERING INFORMATION:


	Size	Code
	545 x 255 mm	ST-394-01
	545 x 255 x 30 mm	ST-394-02

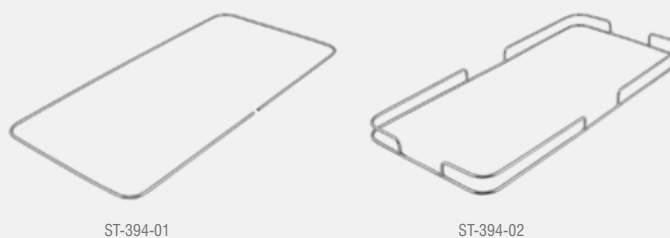

Surticon™ Sterile 1/1 Silicone Mat

ORDERING INFORMATION:

	Size	Code
	450 x 235 mm	ST-396-01
	500 x 235 mm	ST-396-02

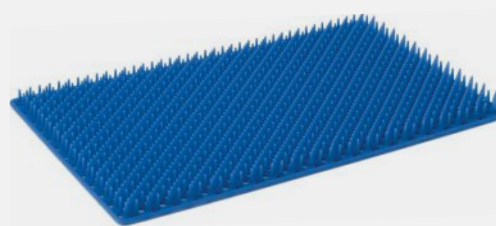


Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System


SurticonTM Sterile Rack for Endoscopic Instruments

ORDERING INFORMATION:

	Size	Code
	10 Instruments	ST-398-01
	20 Instruments	ST-398-02

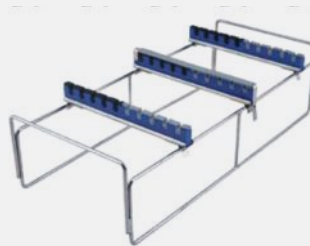

ST-398-01

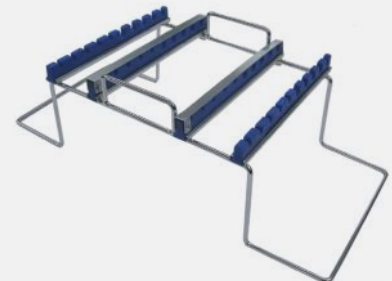


ST-398-02

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 3/4 BioClean™ Sterile Container

Perforated Lid



BioClean™



ST

SURTICON™ STERILE CONTAINER SYSTEM

ORDERING INFORMATION:

465 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-400-01
	Yellow	ST-400-02
	Green	ST-400-03
	Blue	ST-400-04
	Red	ST-400-05
	Black	ST-400-06

465 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-402-01
	Yellow	ST-402-02
	Green	ST-402-03
	Blue	ST-402-04
	Red	ST-402-05
	Black	ST-402-06

465 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-404-01
	Yellow	ST-404-02
	Green	ST-404-03
	Blue	ST-404-04
	Red	ST-404-05
	Black	ST-404-06


465 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-406-01
	Yellow	ST-406-02
	Green	ST-406-03
	Blue	ST-406-04
	Red	ST-406-05
	Black	ST-406-06

465 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-408-01
	Yellow	ST-408-02
	Green	ST-408-03
	Blue	ST-408-04
	Red	ST-408-05
	Black	ST-408-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 3/4 BioClean™ Sterile Container

Perforated Lid & Bottom



BioClean™



ORDERING INFORMATION:

465 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-410-01
	Yellow	ST-410-02
	Green	ST-410-03
	Blue	ST-410-04
	Red	ST-410-05
	Black	ST-410-06

465 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-412-01
	Yellow	ST-412-02
	Green	ST-412-03
	Blue	ST-412-04
	Red	ST-412-05
	Black	ST-412-06

465 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-414-01
	Yellow	ST-414-02
	Green	ST-414-03
	Blue	ST-414-04
	Red	ST-414-05
	Black	ST-414-06

465 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-416-01
	Yellow	ST-416-02
	Green	ST-416-03
	Blue	ST-416-04
	Red	ST-416-05
	Black	ST-416-06


465 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-418-01
	Yellow	ST-418-02
	Green	ST-418-03
	Blue	ST-418-04
	Red	ST-418-05
	Black	ST-418-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

ST

SURTICON™ STERILE CONTAINER SYSTEM

Surticon™ 3/4 BioClean™ Sterile Container (With Safety Lid)
Perforated Lid



BioClean™



ORDERING INFORMATION:

465 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-420-01
	Yellow	ST-420-02
	Green	ST-420-03
	Blue	ST-420-04
	Red	ST-420-05
	Black	ST-420-06

465 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-422-01
	Yellow	ST-422-02
	Green	ST-422-03
	Blue	ST-422-04
	Red	ST-422-05
	Black	ST-422-06

465 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-424-01
	Yellow	ST-424-02
	Green	ST-424-03
	Blue	ST-424-04
	Red	ST-424-05
	Black	ST-424-06

465 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-426-01
	Yellow	ST-426-02
	Green	ST-426-03
	Blue	ST-426-04
	Red	ST-426-05
	Black	ST-426-06

465 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-428-01
	Yellow	ST-428-02
	Green	ST-428-03
	Blue	ST-428-04
	Red	ST-428-05
	Black	ST-428-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 3/4 BioClean™ Sterile Container (With Safety Lid) Perforated Lid & Bottom



BioClean™



ORDERING INFORMATION:

465 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-430-01
	Yellow	ST-430-02
	Green	ST-430-03
	Blue	ST-430-04
	Red	ST-430-05
	Black	ST-430-06

465 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-432-01
	Yellow	ST-432-02
	Green	ST-432-03
	Blue	ST-432-04
	Red	ST-432-05
	Black	ST-432-06

465 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-434-01
	Yellow	ST-434-02
	Green	ST-434-03
	Blue	ST-434-04
	Red	ST-434-05
	Black	ST-434-06

465 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-436-01
	Yellow	ST-436-02
	Green	ST-436-03
	Blue	ST-436-04
	Red	ST-436-05
	Black	ST-436-06

465 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-438-01
	Yellow	ST-438-02
	Green	ST-438-03
	Blue	ST-438-04
	Red	ST-438-05
	Black	ST-438-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 3/4 BioFree™ Sterile Container

Perforated Lid



BioFree™



ORDERING INFORMATION:

465 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-440-01
	Yellow	ST-440-02
	Green	ST-440-03
	Blue	ST-440-04
	Red	ST-440-05
	Black	ST-440-06

465 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-442-01
	Yellow	ST-442-02
	Green	ST-442-03
	Blue	ST-442-04
	Red	ST-442-05
	Black	ST-442-06

465 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-444-01
	Yellow	ST-444-02
	Green	ST-444-03
	Blue	ST-444-04
	Red	ST-444-05
	Black	ST-444-06

465 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-446-01
	Yellow	ST-446-02
	Green	ST-446-03
	Blue	ST-446-04
	Red	ST-446-05
	Black	ST-446-06

465 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-448-01
	Yellow	ST-448-02
	Green	ST-448-03
	Blue	ST-448-04
	Red	ST-448-05
	Black	ST-448-06

ST

SURTICON™ STERILE CONTAINER SYSTEM

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM 3/4 BioFreeTM Sterile Container

Perforated Lid & Bottom



BioFreeTM



ORDERING INFORMATION:

465 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-450-01
	Yellow	ST-450-02
	Green	ST-450-03
	Blue	ST-450-04
	Red	ST-450-05
	Black	ST-450-06

465 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-452-01
	Yellow	ST-452-02
	Green	ST-452-03
	Blue	ST-452-04
	Red	ST-452-05
	Black	ST-452-06

465 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-454-01
	Yellow	ST-454-02
	Green	ST-454-03
	Blue	ST-454-04
	Red	ST-454-05
	Black	ST-454-06

465 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-456-01
	Yellow	ST-456-02
	Green	ST-456-03
	Blue	ST-456-04
	Red	ST-456-05
	Black	ST-456-06


465 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-458-01
	Yellow	ST-458-02
	Green	ST-458-03
	Blue	ST-458-04
	Red	ST-458-05
	Black	ST-458-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

ST

SURTICON™ STERILE CONTAINER SYSTEM

Surticon™ Sterile 3/4 Instrument Basket

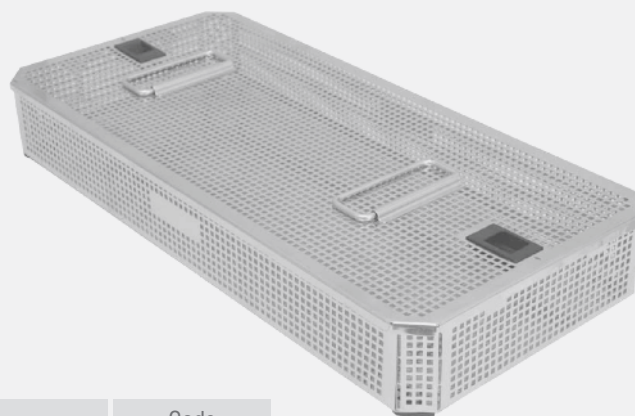

ORDERING INFORMATION:

Without Lid	Size	Code	With Lid	Size	Code
	405 x 252 x 25 mm	ST-480-01		409 x 256 x 25 mm	ST-482-01
	405 x 252 x 45 mm	ST-480-02		409 x 256 x 45 mm	ST-482-02
	405 x 252 x 65 mm	ST-480-03		409 x 256 x 65 mm	ST-482-03
	405 x 252 x 95 mm	ST-480-04		409 x 256 x 95 mm	ST-482-04

Surticon™ Sterile 1/1 Wire Mesh Basket



ORDERING INFORMATION:


Without Lid	Size	Code	With Lid	Size	Code
	405 x 253 x 30 mm	ST-484-01		405 x 253 x 30 mm	ST-486-01
	405 x 253 x 50 mm	ST-484-02		405 x 253 x 50 mm	ST-486-02
	405 x 253 x 70 mm	ST-484-03		405 x 253 x 70 mm	ST-486-03
	405 x 253 x 100 mm	ST-484-04		405 x 253 x 100 mm	ST-486-04

Sterile Container System
 Sterilcontainer System
 Sistema de recipiente estéril
 Système de récipient stérile
 Sterili Container System

Surticon™ Sterile 3/4 Divider

ORDERING INFORMATION:


2 Partitions	Size	Code
	405 x 250 x 80 mm	ST-490-01
	405 x 250 x 110 mm	ST-490-02
	405 x 250 x 130 mm	ST-490-03
3 Partitions	Size	Code
	405 x 250 x 80 mm	ST-492-01
	405 x 250 x 110 mm	ST-492-02
	405 x 250 x 130 mm	ST-492-02

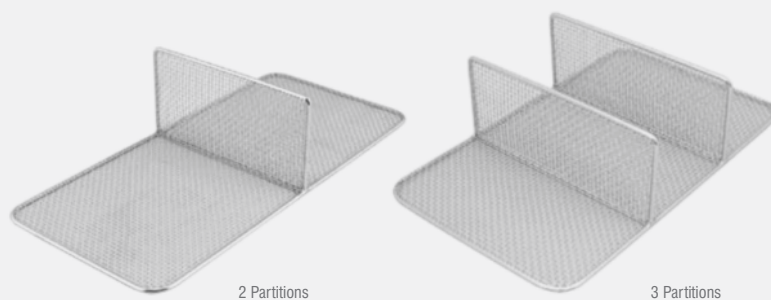

Surticon™ Sterile 3/4 Drape Retainer

ORDERING INFORMATION:


	Size	Code
	405 x 255 mm	ST-494-01
	405 x 255 x 30 mm	ST-494-02

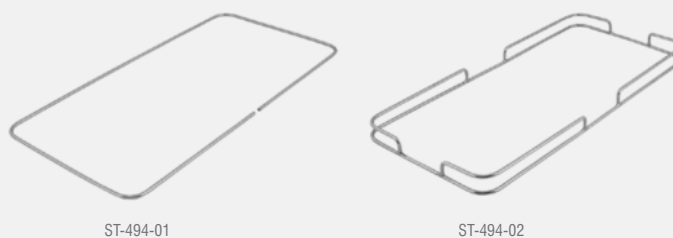

Surticon™ Sterile 3/4 Silicone Mat


ORDERING INFORMATION:

	Size	Code
	370 x 235 mm	ST-496-01

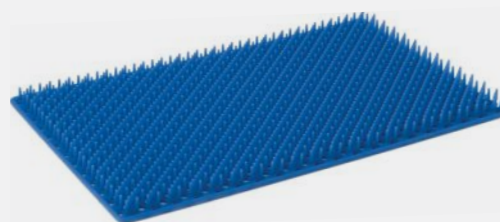

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 1/2 BioClean™ Sterile Container
Perforated Lid



BioClean™



ST

SURTICON™ STERILE CONTAINER SYSTEM

ORDERING INFORMATION:

295 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-500-01
	Yellow	ST-500-02
	Green	ST-500-03
	Blue	ST-500-04
	Red	ST-500-05
	Black	ST-500-06

295 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-502-01
	Yellow	ST-502-02
	Green	ST-502-03
	Blue	ST-502-04
	Red	ST-502-05
	Black	ST-502-06

295 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-504-01
	Yellow	ST-504-02
	Green	ST-504-03
	Blue	ST-504-04
	Red	ST-504-05
	Black	ST-504-06


295 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-506-01
	Yellow	ST-506-02
	Green	ST-506-03
	Blue	ST-506-04
	Red	ST-506-05
	Black	ST-506-06

295 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-508-01
	Yellow	ST-508-02
	Green	ST-508-03
	Blue	ST-508-04
	Red	ST-508-05
	Black	ST-508-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 1/2 BioClean™ Sterile Container

Perforated Lid & Bottom



BioClean™



ORDERING INFORMATION:

255 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-510-01
	Yellow	ST-510-02
	Green	ST-510-03
	Blue	ST-510-04
	Red	ST-510-05
	Black	ST-510-06

295 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-512-01
	Yellow	ST-512-02
	Green	ST-512-03
	Blue	ST-512-04
	Red	ST-512-05
	Black	ST-512-06

295 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-514-01
	Yellow	ST-514-02
	Green	ST-514-03
	Blue	ST-514-04
	Red	ST-514-05
	Black	ST-514-06

295 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-516-01
	Yellow	ST-516-02
	Green	ST-516-03
	Blue	ST-516-04
	Red	ST-516-05
	Black	ST-516-06


295 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-518-01
	Yellow	ST-518-02
	Green	ST-518-03
	Blue	ST-518-04
	Red	ST-518-05
	Black	ST-518-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 1/2 BioClean™ Sterile Container (With Safety Lid)
Perforated Lid



BioClean™

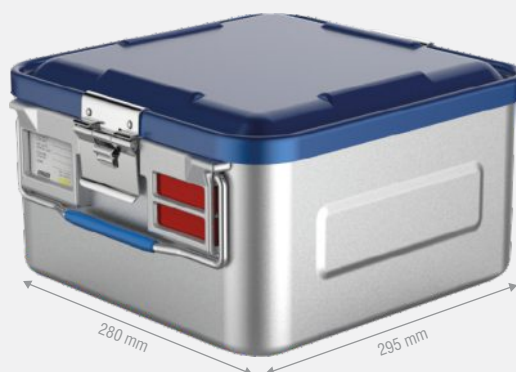

ORDERING INFORMATION:

295 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-520-01
	Yellow	ST-520-02
	Green	ST-520-03
	Blue	ST-520-04
	Red	ST-520-05
	Black	ST-520-06

295 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-522-01
	Yellow	ST-522-02
	Green	ST-522-03
	Blue	ST-522-04
	Red	ST-522-05
	Black	ST-522-06

295 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-524-01
	Yellow	ST-524-02
	Green	ST-524-03
	Blue	ST-524-04
	Red	ST-524-05
	Black	ST-524-06

295 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-526-01
	Yellow	ST-526-02
	Green	ST-526-03
	Blue	ST-526-04
	Red	ST-526-05
	Black	ST-526-06

295 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-528-01
	Yellow	ST-528-02
	Green	ST-528-03
	Blue	ST-528-04
	Red	ST-528-05
	Black	ST-528-06

ST


SURTICON™ STERILE CONTAINER SYSTEM

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 1/2 BioClean™ Sterile Container (With Safety Lid) Perforated Lid & Bottom



BioClean™

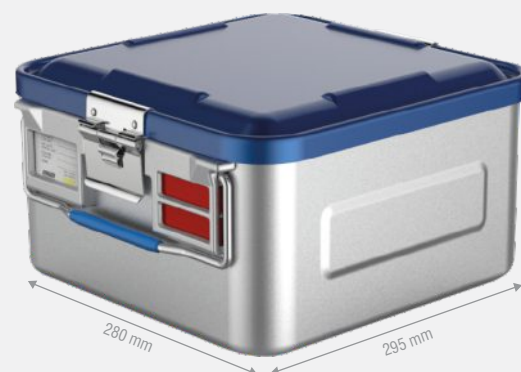

ORDERING INFORMATION:

295 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-530-01
	Yellow	ST-530-02
	Green	ST-530-03
	Blue	ST-530-04
	Red	ST-530-05
	Black	ST-530-06

295 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-532-01
	Yellow	ST-532-02
	Green	ST-532-03
	Blue	ST-532-04
	Red	ST-532-05
	Black	ST-532-06

295 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-534-01
	Yellow	ST-534-02
	Green	ST-534-03
	Blue	ST-534-04
	Red	ST-534-05
	Black	ST-534-06

295 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-536-01
	Yellow	ST-536-02
	Green	ST-536-03
	Blue	ST-536-04
	Red	ST-536-05
	Black	ST-536-06

295 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-538-01
	Yellow	ST-538-02
	Green	ST-538-03
	Blue	ST-538-04
	Red	ST-538-05
	Black	ST-538-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 1/2 BioFree™ Sterile Container

Perforated Lid



BioFree™



ST

SURTICON™ STERILE CONTAINER SYSTEM

ORDERING INFORMATION:

295 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-540-01
	Yellow	ST-540-02
	Green	ST-540-03
	Blue	ST-540-04
	Red	ST-540-05
	Black	ST-540-06

295 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-542-01
	Yellow	ST-542-02
	Green	ST-542-03
	Blue	ST-542-04
	Red	ST-542-05
	Black	ST-542-06

295 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-544-01
	Yellow	ST-544-02
	Green	ST-544-03
	Blue	ST-544-04
	Red	ST-544-05
	Black	ST-544-06

295 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-546-01
	Yellow	ST-546-02
	Green	ST-546-03
	Blue	ST-546-04
	Red	ST-546-05
	Black	ST-546-06

295 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-548-01
	Yellow	ST-548-02
	Green	ST-548-03
	Blue	ST-548-04
	Red	ST-548-05
	Black	ST-548-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 1/2 BioFree™ Sterile Container

Perforated Lid & Bottom



BioFree™



ORDERING INFORMATION:

295 x 280 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-550-01
	Yellow	ST-550-02
	Green	ST-550-03
	Blue	ST-550-04
	Red	ST-550-05
	Black	ST-550-06

295 x 280 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-552-01
	Yellow	ST-552-02
	Green	ST-552-03
	Blue	ST-552-04
	Red	ST-552-05
	Black	ST-552-06

295 x 280 x 155 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-554-01
	Yellow	ST-554-02
	Green	ST-554-03
	Blue	ST-554-04
	Red	ST-554-05
	Black	ST-554-06

295 x 280 x 205 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-556-01
	Yellow	ST-556-02
	Green	ST-556-03
	Blue	ST-556-04
	Red	ST-556-05
	Black	ST-556-06

295 x 280 x 265 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-558-01
	Yellow	ST-558-02
	Green	ST-558-03
	Blue	ST-558-04
	Red	ST-558-05
	Black	ST-558-06

Sterile Container System
 Sterilcontainer System
 Sistema de recipiente estéril
 Système de récipient stérile
 Sterili Container System

ST

SURTICON™ STERILE CONTAINER SYSTEM

Surticon™ Sterile 1/2 Instrument Basket



ORDERING INFORMATION:

Without Lid	Size	Code	With Lid	Size	Code
	242x 252 x 25 mm	ST-585-01		246 x 256 x 25 mm	ST-582-01
	242 x 252 x 45 mm	ST-585-02		246 x 256 x 45 mm	ST-582-02
	242 x 252 x 65 mm	ST-585-03		246 x 256 x 65 mm	ST-582-03
	242 x 252 x 95 mm	ST-585-04		246 x 256 x 95 mm	ST-582-04

Surticon™ Sterile 1/2 Wire Mesh Basket



ORDERING INFORMATION:

Without Lid	Size	Code	With Lid	Size	Code
	255 x 250 x 30 mm	ST-584-01		255 x 250 x 30 mm	ST-586-01
	255 x 250 x 50 mm	ST-584-02		255 x 250 x 50 mm	ST-586-02
	255 x 250 x 70 mm	ST-584-03		255 x 250 x 70 mm	ST-586-03
	255 x 250 x 100 mm	ST-584-04		255 x 250 x 100 mm	ST-586-04




Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM Sterile 1/2 Wire Base

ORDERING INFORMATION:


	Size	Code
	255 x 255 x 30 mm	ST-588-01

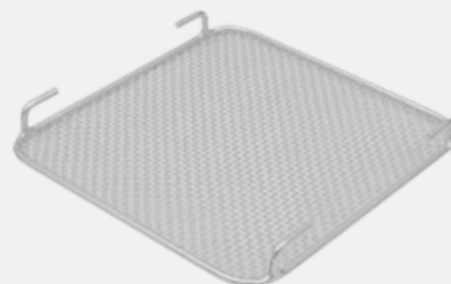

SurticonTM Sterile 3/4 Divider

ORDERING INFORMATION:

4 Partitions	Size	Code
	255 x 245 x 130 mm	ST-590-01
	255 x 245 x 180 mm	ST-590-02

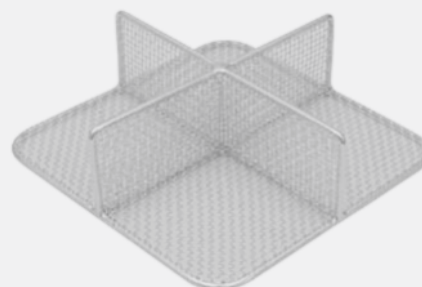

4 Partitions


SurticonTM Sterile 3/4 Divider

ORDERING INFORMATION:

4 Partitions	Size	Code
	255 x 255 mm	ST-594-01
	255 x 255 mm	ST-594-02



ST-594-01

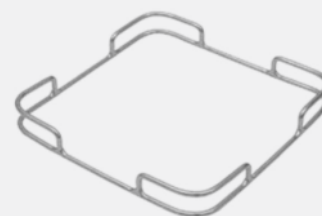


ST-594-02

SurticonTM Sterile 1/2 Silicone Mat

ORDERING INFORMATION:

	Size	Code
	255 x 255 mm	ST-596-01

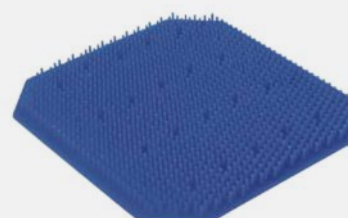

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM Sterile 1/2 Wire Base

ORDERING INFORMATION:

	Size	Code
	Standard	ST-598-01





ST

SURTICONTM STERILE CONTAINER SYSTEM

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ Sterile Container Dental Model

Perforated Lid

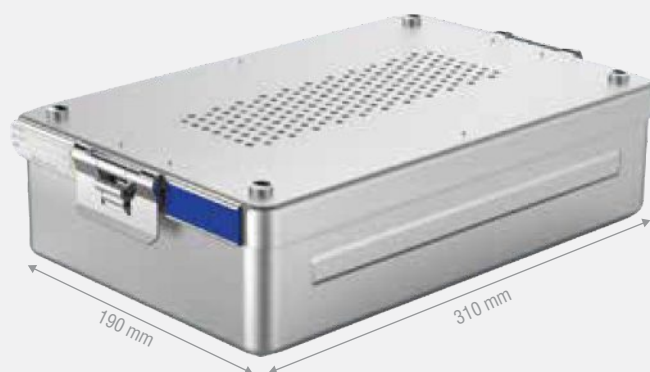

ORDERING INFORMATION:


310 x 190 x 45 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-600-01
	Yellow	ST-600-02
	Green	ST-600-03
	Blue	ST-600-04
	Red	ST-600-05
	Black	ST-600-06

310 x 190 x 65 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-602-01
	Yellow	ST-602-02
	Green	ST-602-03
	Blue	ST-602-04
	Red	ST-602-05
	Black	ST-602-06

310 x 190 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-604-01
	Yellow	ST-604-02
	Green	ST-604-03
	Blue	ST-604-04
	Red	ST-604-05
	Black	ST-604-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ 1/1 Sterile Container Dental Model
Perforated Lid and Bottom

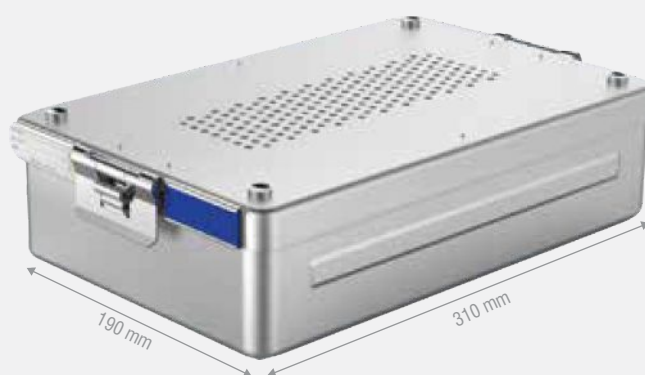

ORDERING INFORMATION:

310 x 190 x 45 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-610-01
	Yellow	ST-610-02
	Green	ST-610-03
	Blue	ST-610-04
	Red	ST-610-05
	Black	ST-610-06

310 x 190 x 65 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-612-01
	Yellow	ST-612-02
	Green	ST-312-03
	Blue	ST-312-04
	Red	ST-312-05
	Black	ST-312-06

310 x 190 x 135 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-614-01
	Yellow	ST-614-02
	Green	ST-614-03
	Blue	ST-614-04
	Red	ST-614-05
	Black	ST-614-06

ST


SURTICON™ STERILE CONTAINER SYSTEM

Sterile Container System
 Sterilcontainer System
 Sistema de recipiente estéril
 Système de récipient stérile
 Sterili Container System

ST

SURTICON™ STERILE CONTAINER SYSTEM


Surticon™ Sterile Dental Model Wire Mesh Basket Without Lid

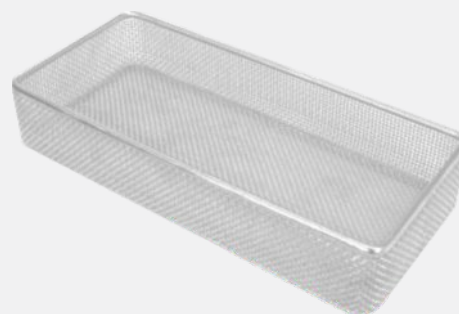

ORDERING INFORMATION:

	Size	Code
	274 x 172 x 43 mm	ST-680-01


Surticon™ Sterile Dental Model Wire Mesh Basket With Lid

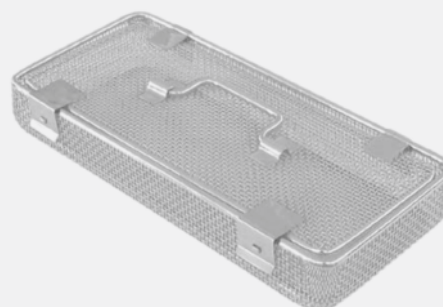

ORDERING INFORMATION:

	Size	Code
	274 x 172 x 43 mm	ST-682-01


Surticon™ Sterile Dental Model Drape Retainer

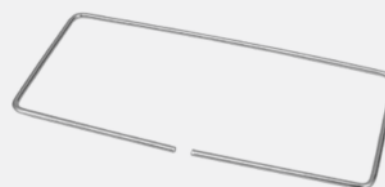

ORDERING INFORMATION:

	Size	Code
	277 x 175 mm	ST-694-01

Surticon™ Sterile Dental Model Silicone Mat

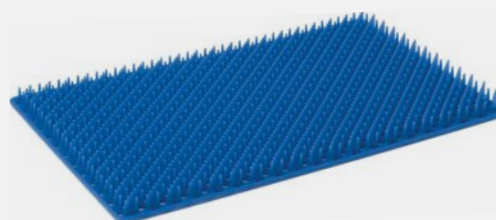

ORDERING INFORMATION:

	Size	Code
	260 x 180 mm	ST-696-01



Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ Sterile Dental Model Single-Use Paper Filter
With Indicator (Pack of 100)

ORDERING INFORMATION:

	Size	Code
	Dental Model Size	ST-698-01



Surticon™ Sterile Dental Model Reusable Teflon Filter


ORDERING INFORMATION:

	Size	Code
	Dental Model Size	ST-698-02



Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM Sterile Container Mini Model
Perforated Lid



ST

SURTICONTM STERILE CONTAINER SYSTEM

ORDERING INFORMATION:

310 x 140 x 45 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-700-01
	Yellow	ST-700-02
	Green	ST-700-03
	Blue	ST-700-04
	Red	ST-700-05
	Black	ST-700-06

310 x 140 x 75 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-702-01
	Yellow	ST-702-02
	Green	ST-702-03
	Blue	ST-702-04
	Red	ST-702-05
	Black	ST-702-06

310 x 140 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-704-01
	Yellow	ST-704-02
	Green	ST-704-03
	Blue	ST-704-04
	Red	ST-704-05
	Black	ST-704-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ Sterile Container Mini Model

Perforated Lid and Bottom



ORDERING INFORMATION:

310 x 140 x 45 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-710-01
	Yellow	ST-710-02
	Green	ST-710-03
	Blue	ST-710-04
	Red	ST-710-05
	Black	ST-710-06

310 x 140 x 75 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-712-01
	Yellow	ST-712-02
	Green	ST-712-03
	Blue	ST-712-04
	Red	ST-712-05
	Black	ST-712-06


310 x 140 x 105 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-714-01
	Yellow	ST-714-02
	Green	ST-714-03
	Blue	ST-714-04
	Red	ST-714-05
	Black	ST-714-06

Sterile Container System
 Sterilcontainer System
 Sistema de recipiente estéril
 Système de récipient stérile
 Sterili Container System

ST

SURTICON™ STERILE CONTAINER SYSTEM


Surticon™ Sterile Mini Model Wire Mesh Basket Without Lid

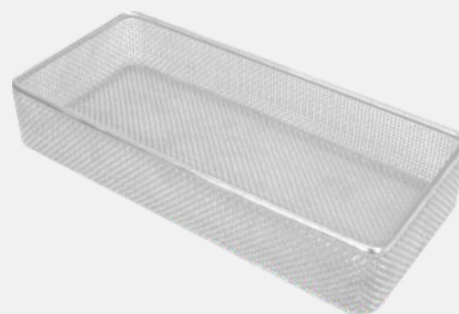

ORDERING INFORMATION:

	Size	Code
	267 x 125 x 50 mm	ST-780-01


Surticon™ Sterile Mini Model Wire Mesh Basket With Lid

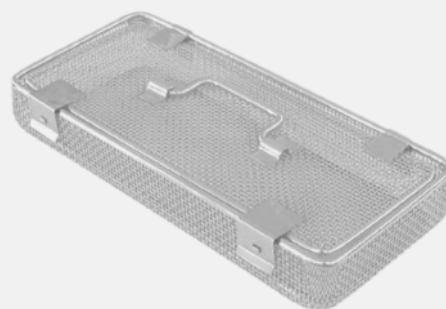

ORDERING INFORMATION:

	Size	Code
	267 x 125 x 50 mm	ST-782-01


Surticon™ Sterile Mini Model Wire Mesh Base

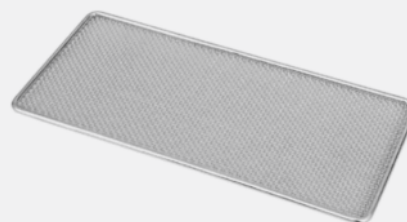

ORDERING INFORMATION:

	Size	Code
	270 x 125 mm	ST-788-01

Surticon™ Sterile Mini Model Drape Retainer

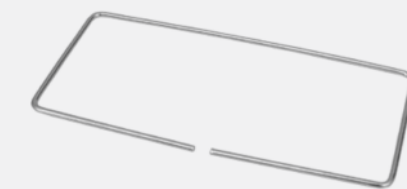

ORDERING INFORMATION:


	Size	Code
	270 x 125 mm	ST-794-01

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM Sterile Mini Model Silicone Mat

ORDERING INFORMATION:

Size	Code
270 x 125 mm	ST-796-01

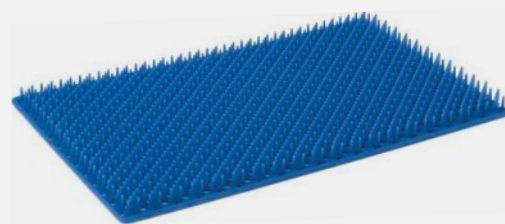

SurticonTM Sterile Mini Model Single-Use Paper Filter With Indicator (Pack of 100)

ORDERING INFORMATION:

Size	Code
Dental Model Size	ST-798-01



SurticonTM Sterile Mini Model Reusable Teflon Filter

ORDERING INFORMATION:


Size	Code
Dental Model Size	ST-798-02



Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ Sterile Container Implant Model

Perforated Lid



ST-800-01

ST-802-01

ORDERING INFORMATION:

310 x 140 x 65 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-800-01
	Yellow	ST-800-02
	Green	ST-800-03
	Blue	ST-800-04
	Red	ST-800-05
	Black	ST-800-06

500 x 155 x 75 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-802-01
	Yellow	ST-802-02
	Green	ST-802-03
	Blue	ST-802-04
	Red	ST-802-05
	Black	ST-802-06

ST

SURTICON™ STERILE CONTAINER SYSTEM

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ Sterile Container Implant Model

Perforated Lid and Bottom



ST-810-01

ST-812-01

ORDERING INFORMATION:



310 x 140 x 65 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-810-01
	Yellow	ST-810-02
	Green	ST-810-03
	Blue	ST-810-04
	Red	ST-810-05
	Black	ST-810-06

500 x 155 x 75 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-812-01
	Yellow	ST-812-02
	Green	ST-812-03
	Blue	ST-812-04
	Red	ST-812-05
	Black	ST-812-06

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ Sterile Container Scopy Model

Perforated Lid

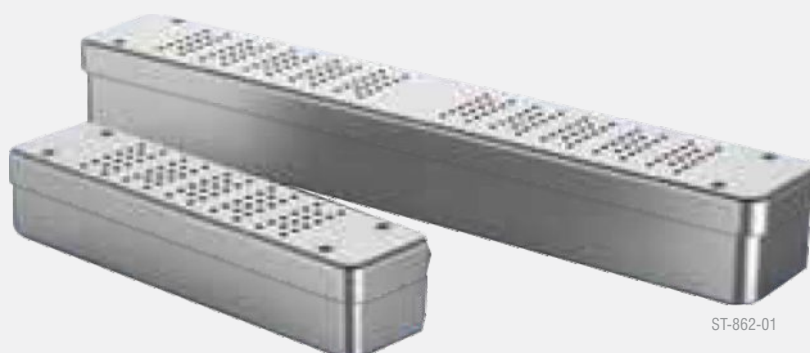

ST-860-01

ST-862-01

ORDERING INFORMATION:

250 x 60 x 50 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-860-01
	Yellow	ST-860-02
	Green	ST-860-03
	Blue	ST-860-04
	Red	ST-860-05
	Black	ST-860-06

450 x 70 x 70 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-862-01
	Yellow	ST-862-02
	Green	ST-862-03
	Blue	ST-862-04
	Red	ST-862-05
	Black	ST-862-06



ST

SURTICON™ STERILE CONTAINER SYSTEM

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM Sterile Container Scopy Model

Perforated Lid and Bottom

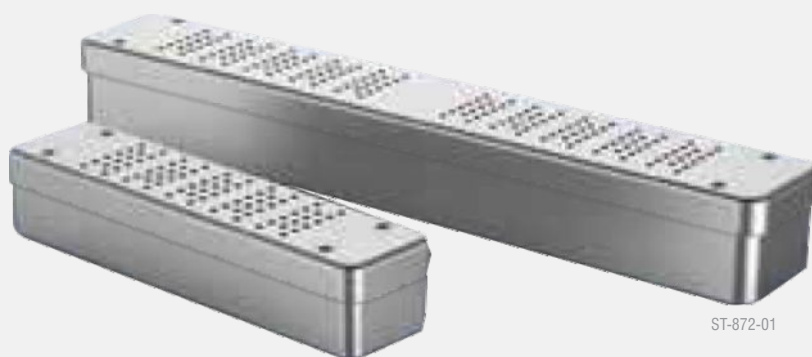

ST-870-01

ST-872-01

ORDERING INFORMATION:

250 x 60 x 50 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-870-01
	Yellow	ST-870-02
	Green	ST-870-03
	Blue	ST-870-04
	Red	ST-870-05
	Black	ST-870-06

450 x 70 x 70 mm (Length x Width x Height)	Lid Color	Code
	Grey	ST-872-01
	Yellow	ST-872-02
	Green	ST-872-03
	Blue	ST-872-04
	Red	ST-872-05
	Black	ST-872-06

Sterilizing Cases and Accessories
 Sterilisierbehälter Koffer und Zubehör
 Los casos de esterilización y accesorios
 Stérilisation cas et accessoires
 Sterilizzazione Custodie e accessori

Surticon™ Sterile Single-Use Paper Filter

For 1/1-3/4-1/2 Containers-With Indicator (Pack of 100)

ORDERING INFORMATION:

Size	Code
1/1, 3/4, 1/2 Size	ST-900-01



Surticon™ Sterile Reusable Teflon Filter

For 1/1-3/4-1/2 Containers

ORDERING INFORMATION:

Size	Code
1/1, 3/4, 1/2 Size	ST-900-02




Surticon™ Sterile Instrument Basket Stand

ORDERING INFORMATION:

Size	Code
20 mm	ST-902-01
14 mm	ST-902-02



ST-902-01
20 mm



ST-902-02
14 mm

Surticon™ Sterile Security Seal

With Indicator (Pack of 100)

ORDERING INFORMATION:

Size	Code
Blue	ST-905-01
Red	ST-905-02



ST

SURTICON™ STERILE CONTAINER SYSTEM

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ Sterile Security Seal

Non-Indicator (Pack of 100)

ORDERING INFORMATION:

Size	Code
Blue	ST-907-01
Red	ST-907-02

Surticon™ Sterile Paper Label

With Indicator (Pack of 100)

ORDERING INFORMATION:

Size	Code
Small	ST-910-01
Large	ST-910-02



Sterilizing Cases and Accessories
Sterilisierbehälter Koffer und Zubehör
Los casos de esterilización y accesorios
Stérilisation cas et accessoires
Sterilizzazione Custodie e accessori

ST

SURTICON™ STERILE CONTAINER SYSTEM

Surticon™ Sterile Identification Label

16 Letter-Engraved to Specifications

ORDERING INFORMATION:

Size	Code
Grey	ST-914-01
Yellow	ST-914-02
Green	ST-914-03
Blue	ST-914-04
Red	ST-914-05
Black	ST-914-06



Surticon™ Sterile Holder for Identification Label

ORDERING INFORMATION:

Size	Code
50 x 35 x 13	ST-916-01



Surticon™ Sterile Silicone Handle

ORDERING INFORMATION:


Size	Code
Grey	ST-920-01
Yellow	ST-920-02
Green	ST-920-03
Blue	ST-920-04
Red	ST-920-05
Black	ST-920-06



Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM Sterile Fixation Clamp

ORDERING INFORMATION:

	Size	Code
	Standard	ST-796-01




Sterilizing Cases and Accessories
 Sterilisierbehälter Koffer und Zubehör
 Los casos de esterilización y accesorios
 Stérilisation cas et accessoires
 Sterilizzazione Custodie e accessori

ST

SurticonTM Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
97 x 41 mm	ST-960-01
136 x 41 mm	ST-960-02
164 x 41 mm	ST-960-03
250 x 41 mm	ST-960-04

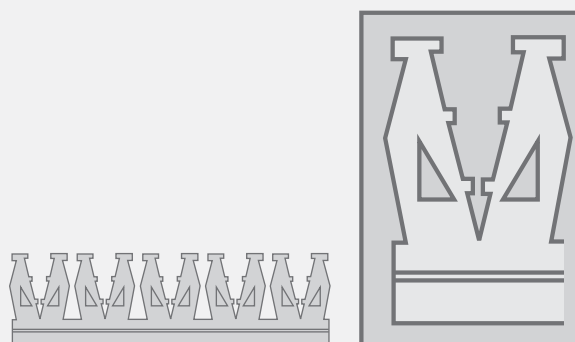

SurticonTM Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
90 x 41 mm	ST-962-01
130 x 41 mm	ST-962-02
160 x 41 mm	ST-962-03
240 x 41 mm	ST-962-04

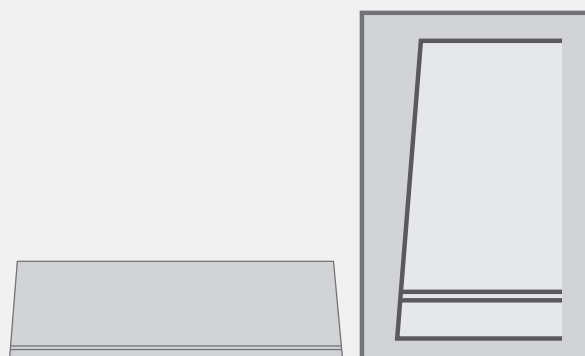

SurticonTM Sterile Silicone Fixation System

ORDERING INFORMATION:

Size	Code
87 x 41 mm	ST-964-01
144 x 41 mm	ST-964-02
175 x 41 mm	ST-585-03
238 x 41 mm	ST-585-04


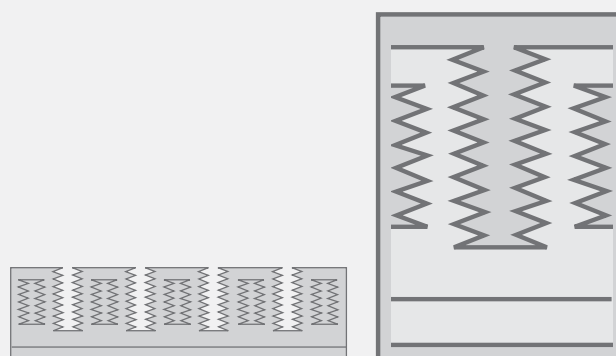

 SURTICONTM STERILE CONTAINER SYSTEM

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
77 x 41 mm	ST-966-01
127 x 41 mm	ST-966-02
162 x 41 mm	ST-966-03
250 x 41 mm	ST-966-04

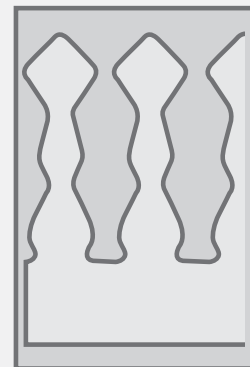

Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:

Size	Code
178 x 20 mm	ST-968-01



Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:

Size	Code
72 x 20 mm	ST-970-01



Sterilizing Cases and Accessories
 Sterilisierbehälter Koffer und Zubehör
 Los casos de esterilización y accesorios
 Stérilisation cas et accessoires
 Sterilizzazione Custodie e accessori


ST

SURTICON™ STERILE CONTAINER SYSTEM

Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
72 x 20 mm	ST-972-01

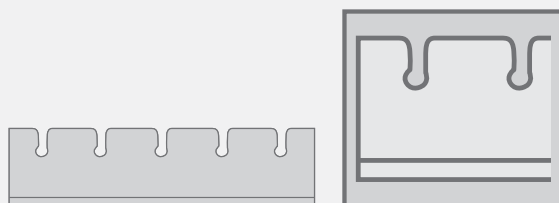

Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
178 x 30 mm	ST-974-01

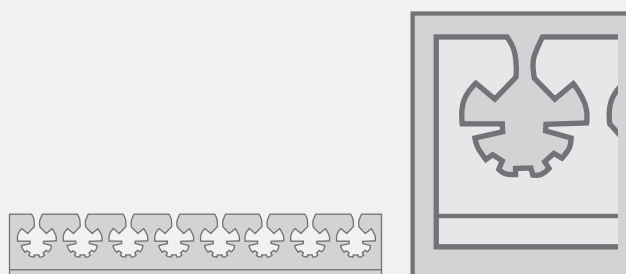

Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
121 x 18 mm	ST-976-01

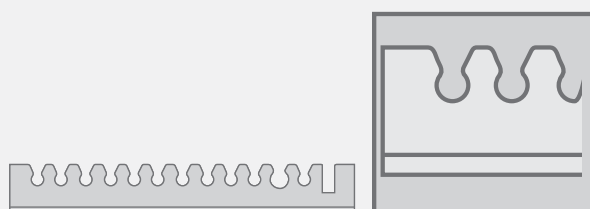

Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:

Size	Code
123 x 18 mm	ST-978-01

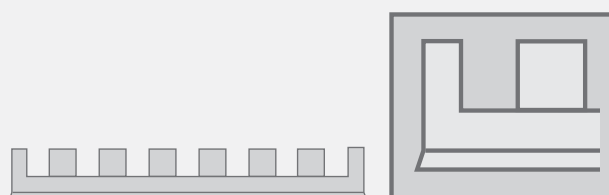


Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System

SurticonTM Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
123 x 18 mm	ST-980-01



SurticonTM Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
178 x 20 mm	ST-982-01



SurticonTM Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
178 x 20 mm	ST-984-01



Sterilizing Cases and Accessories
 Sterilisierbehälter Koffer und Zubehör
 Los casos de esterilización y accesorios
 Stérilisation cas et accessoires
 Sterilizzazione Custodie e accessori

ST
SURTICON™ STERILE CONTAINER SYSTEM


Surticon™ Sterile Silicone Fixation System

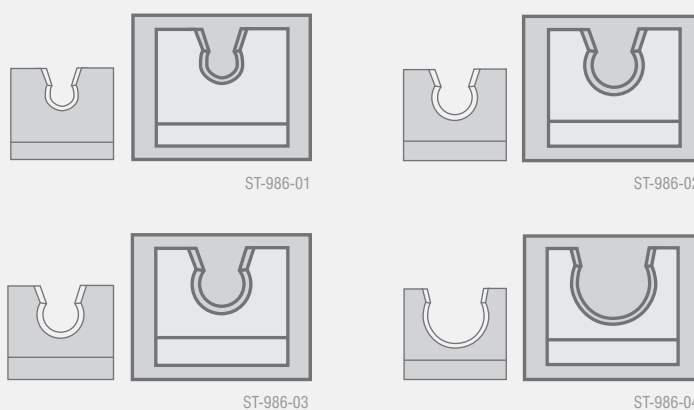

ORDERING INFORMATION:

Size	Code
23.5 x 21 mm	ST-986-01
23.5 x 21 mm	ST-986-02
23.5 x 21 mm	ST-986-03
23.5 x 21 mm	ST-986-04

Surticon™ Sterile Silicone Fixation System

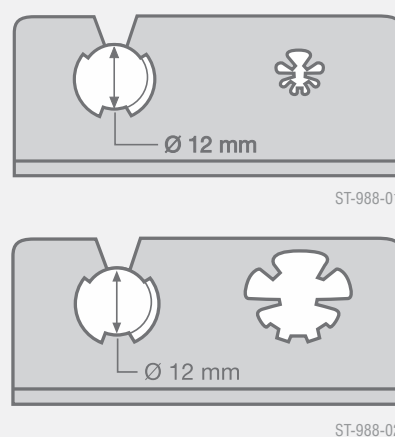

ORDERING INFORMATION:


Size	Code
72 x 30 mm	ST-988-01
72 x 30 mm	ST-988-02

Sterile Container System
Sterilcontainer System
Sistema de recipiente estéril
Système de récipient stérile
Sterili Container System


Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:

Size	Code
38 x 30 mm	ST-990-01
72 x 30 mm	ST-990-03



ST-990-01

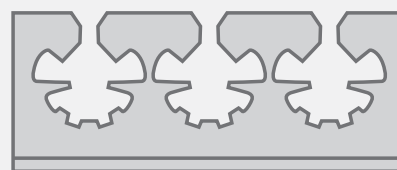


ST-990-03


Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:

Size	Code
38 x 30 mm	ST-992-01
72 x 30 mm	ST-992-03



ST-992-01

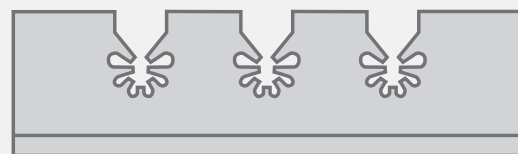


ST-992-03


Surticon™ Sterile Silicone Fixation System

ORDERING INFORMATION:


Size	Code
38 x 29 mm	ST-994-01
38 x 29 mm	ST-994-02
38 x 29 mm	ST-994-03
38 x 29 mm	ST-994-04



ST-994-01



ST-994-02



ST-994-03




ST-994-04

Sterilizing Cases and Accessories
Sterilisierbehälter Koffer und Zubehör
Los casos de esterilización y accesorios
Stérilisation cas et accessoires
Sterilizzazione Custodie e accessori

SurticonTM Sterile Silicone Fixation System

ORDERING INFORMATION:

Size	Code
38 x 29 mm	ST-996-01
38 x 29 mm	ST-996-02

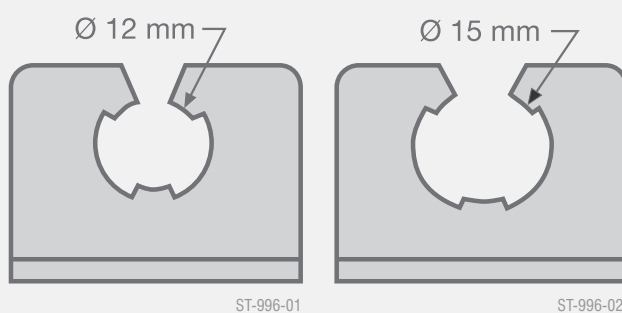

ST

SURTICONTM STERILE CONTAINER SYSTEM

General Terms and Conditions of Sales

1. Definitions

“**Company**” means Surtex Instruments Ltd (registered in the United Kingdom under number 7035724).

“**Contract**” means the Order accepted by the Company and incorporating these conditions.

“**Customer**” means the company, firm or organisation who's Order for the Goods is accepted by the Company.

“**Goods**” means the goods which the Company agrees to supply in accordance with these conditions and which are identified on the Order. “**Order**” means the order for the purchase of the Goods submitted by the Customer.

“**Goods**” means the goods agreed to be provided to the customs by Surtex Instrument Ltd.

“**Quotation**” means the quotation by Surtex Instruments stating the price at which and the time period during which it will supply the goods to the customer.

1. Any reference to a law is a reference to it as in force for the time being taking account of any amendment, extension, application or re-enactment and includes any subordinate legislation for the time being in force made under it.
2. Where a condition provides for a list of items following the word “including” or “includes”, then such list is not to be interpreted as being an exhaustive list.

2. General

- 2.1 Headings are purely for the ease of reference and do not form part of effect the interpretation of Conditions.
- 2.2 In the event of a conflict the contractual documents shall be applied in the following order:
 - a) the Quotation
 - b) the Conditions
- 2.3 No other terms and conditions or warranted are to be incorporated into the Contract unless agreed expressly in writing with Surtex Instruments. In particular, the Customer's terms and conditions are expressly excluded whether provided in full, referred to in other documents and whether before or after the Contract is formed.
- 2.4 Surtex Instruments may update or amend these Conditions from time to time to comply with the law or to meet the changing business requirements without notice to the customer.

3. Ordering

- 3.1 Each Order (whether submitted by telephone, fax, post, email or electronic ordering system) shall be deemed to be an offer by the Customer to purchase the Goods pursuant to these conditions. The Company may, at its complete discretion, refuse to accept any Order. The Contract will be formed upon confirmation of acceptance of the Customer's purchase order by Surtex Instruments.
- 3.2 The Customer shall be responsible to the Company for ensuring the accuracy of the terms of any Order (including the description of the Goods ordered).

Samples and Free of Charge Goods

- 3.3 For the avoidance of doubt, where no order is placed and the Company provides Samples, to familiarize the Customer with the goods, as part of a sampling program or where the Company provides Free of Charge Goods to the Customer as part of a clinical trial or compassionate use program these conditions shall, to the extent applicable, apply to such Samples and Free of Charge Goods.

4. Prices

- 4.1 The price is exclusive of VAT and all other applicable taxes and duties, which the Customer shall be additionally liable to pay the Surtex Instruments.
- 4.2 All prices quoted are subject to change up to the date of delivery, subject to prior written notice by Surtex Instruments.
- 4.3 Surtex Instruments reserves the right, by giving notice to the Customer at any time before delivery, to increase the price of the Goods to reflect any increase in the cost of Surtex Instruments which is due to any factor beyond the reasonable control of Surtex Instruments.
- 4.4 Errors on Surtex Instruments website prices and availability of products and services are subject to change without notice errors will be corrected where discovered, and Surtex Instruments reserves the right to revoke any stated offer and to correct any errors, inaccuracies or omissions including after an order has been submitted and whether or not the order has been confirmed and your credit card charged. Surtex Instruments shall have the right to refuse or cancel any orders placed for product listed at the incorrect price. Surtex Instruments shall have the right to refuse or cancel any such orders whether or not the order has been confirmed and your credit card charged. If your credit card has already been charged for the purchase and your order is cancelled, Surtex Instruments will issue a credit to your credit card account in the amount of the charge. Individual bank policies will dictate when this amount is credited to your account. If you are not fully satisfied with your purchase, you may return it in accordance with Surtex Instruments' Return Policy.

5. Delivery

- 5.1 Delivery of the Goods shall be made to the delivery address specified as stated on the Pro Forma Invoice or communicated separately whichever is greater after the date of the Surtex Instruments acceptance of the Order.
- 5.2 Surtex Instruments reserves the right to withhold delivery of any Goods if any sum due under any contract with the Customer is overdue or if, in the reasonable opinion of Surtex Instruments, the financial standing of the Customer has been impaired for any other reason.
- 5.3 Time for delivery shall not be of the essence and, Surtex Instruments shall not be liable for any loss or damage whatever due to any failure by the Surtex Instruments to deliver the Goods (or any of them) promptly or at all. The customer will have no right damages or to cancel the order for any failure to meet the delivery times stated.
- 5.4 The delivery of the Goods may happen by separate instalments. Each separate instalment shall be invoiced and paid for in accordance with the provisions of the Contract. Each instalment shall be a separate Contract and no cancellation or termination of any one Contract relating to an instalment shall entitle the Customer to repudiate or cancel any other Contractor instalment.
- 5.5 The Customer shall take delivery of the Goods promptly whenever they are tendered for delivery (which shall include signing the relevant delivery note) If, for any reason, the Customer fails to take such delivery of the Goods or otherwise causes or requests a delay in delivery:
 - a) The Goods shall be deemed to have been delivered;
 - b) Risk in the Goods shall pass to the Customer, and
 - c) Surtex Instruments shall be entitled to store or arrange for the storage of the Goods until actual delivery and charge the Customer for the reasonable costs (including insurance) of such storage and any additional charges incurred in delivering the Goods at a later date.
- 5.6 The Customer shall ensure that adequate and safe facilities and procedures exist at the Customer's premises for the delivery of the Goods.
- 5.7 The Customer shall immediately notify Surtex Instruments Customer Support Centre if the Goods are not received within 10 days of the specified delivery date.
- 5.8 The customer outside of the UK shall be solely responsible for obtaining all import authorisations.

6. Title and Risk

- 6.1 The Goods shall be at the Customer's risk at the time of delivery unless the parties have agreed in writing that the Goods are to be collected from the Surtex Instruments premises, in which case, the Goods shall be at the Customer's risk when Surtex Instruments notifies the Customer that the Goods are available for collection.
 1. Property in the Goods shall not pass from Surtex Instruments until:
 - a) The Customer has paid the price in full; and
 - b) No other sums whatsoever are due from the Customer to Surtex Instruments.

2. Until property in the Goods passes to the Customer in accordance with the condition 6.1, the Customer shall:

- a) Hold the Goods on a fiduciary basis as bailed for Surtex Instruments
- b) Store the Goods separately from all other goods in its possession and mark them in such a way that they are clearly identified as Surtex Instrument's property; and
- c) Maintain the Goods in satisfactory condition and keep them insured on Surtex Instrument's behalf for their full price.

3. The Customer may sell at full market value or use the Goods only in the ordinary course of the Customer's business. Any such sale or dealing shall be a sale or use of Surtex Instrument's property on the Customer's own behalf and the Customer shall deal as principal when making such sales or dealings. Until property in the Goods passes from Surtex Instruments, the proceeds of sale or otherwise of the Goods, to the full extent of the price of the Goods, shall be held in trust for Surtex Instruments and shall not be mixed with other money or paid into any overdrawn bank account and shall be at all material times identified as Surtex Instruments money.

4. Surtex Instruments shall be entitled to recover the price notwithstanding that property in any of the Goods has not passed from Surtex Instruments.

5. Until such time as the property in the Goods passes from Surtex Instruments, if the Customer: a) Enters into liquidation or has a winding-up order made against it or has an administrator, receiver or manager appointed in respect of its assets; or b) Fails to make payment in accordance with these conditions, the Customer shall upon request deliver up Surtex Instruments such of the Goods as have not ceased to be in existence or resold. If the Customer fails to do so, Surtex Instruments may enter upon any premises owned, occupied or controlled by the Customer where the Goods are situated and repossess the Goods.

6. The Customer shall not pledge or in any way charge by way of security for any indebtedness, any of the Goods which are the property Surtex Instruments. If the Customer does so, all sums whatever owing by the Customer to Surtex Instruments shall forthwith become due and payable.

7. On termination of the Contract, howsoever caused, Surtex Instruments rights contained in this condition 6 shall remain in effect.

7. Terms of Payment

7.1 Payment is due to Surtex Instruments within 30 days of invoice (the "Due Date"). In the case of payment other than by cash, payment shall only be deemed to have been made on receipt of cleared funds.

7.2 Each consignment or partial delivery shall be invoiced and paid separately.

7.3 No disputes arising under the contract no delays in the delivery period beyond the control of Surtex Instruments shall interfere with prompt payment in full by Customer. The Customer shall not in any circumstances or for any reason whatsoever be entitled to make any deduction or withhold any sum from the price by way of set-off or otherwise.

7.4 If the Customer fails to make the payment on the due date, then Surtex Instruments without prejudice to other rights and remedies shall be entitled to charge the Customer interest (both before and after judgment) on the amount unpaid at the rate of 4% per annum above the basic rate of HSBC plc during the delay and suspend all further deliveries without notice.

7.5 All payments payable to the Company under the Contract shall become due immediately on its termination, despite any other provision.

8. Warranties

8.1 Surtex Instruments will use reasonable endeavours to ensure that the Goods

- a) Correspond to their description and any applicable specification;
- b) Be of satisfactory quality and fit for purpose held out by Surtex Instruments or made to known to the customer by Surtex Instruments
- c) Where applicable, be free from defects in design, materials and workmanship and remain so for a period of 12 months after delivery; and
- d) Comply with all applicable statutory and regulatory requirements relating to the manufacture, labelling, packaging, storage, handling and delivery of Goods

8.3 In case of Goods not manufactured by Surtex Instruments

- a) Surtex Instruments gives no assurance or warranty whatsoever that the sale or use of the Goods will not infringe the patent design right registered, design copyright or other industrial property rights of other person firm or Company and
- b) The warranty given to the Customer shall be limited to the warranty (if any) which Surtex Instruments receives from the manufacturer or supplier of the Goods to Surtex Instruments.

9. Missing and Defective Goods

9.1 The Customer must inspect the Goods immediately on arrival at their premises.

9.2 In case of missing goods or defects apparent on inspection:

- a) a written complaint must be made to Surtex Instruments by the customer within seven days of receipt of the Goods specifying the shortage and/or defect and
- b) Surtex Instruments shall be given an opportunity to inspect the Goods and investigate any complaint before any use is made of the Goods.

9.3 In the case of defects not apparent on inspection:

- a) the Customer shall send a written complaint to Surtex Instruments as soon as reasonably practicable after the defect is noticed and ensure no use is made of or alterations made to the Goods thereafter;
- b) the Customer shall allow Surtex Instruments 30 days to inspect the Goods and shall take such steps as are necessary to enable Surtex Instruments to do so including returning of the Goods to its head office in the United Kingdom if requested.

9.4 In any potential case of a product being defective pursuant to Part 1 of the Consumer Protection Act 1987, the customer must send the complaint within 12 months of the date of delivery by Surtex Instruments or in the case of items not manufactured by Surtex Instruments, within the guarantee period specified by the manufacturer of such item.

9.5 Any complaints made outside of the periods specified in clause 9 will not be considered.

9.6 All allegations of total non-delivery of any consignment of the Goods must be made by notice in writing by the customer to Surtex Instruments within 10 days of the specified delivery date. Failure by the Customer to give such notice shall render the Customer liable for any temporary or permanent loss of the Goods and all additional costs and expenses incurred by Surtex Instruments in relation to such loss.

10. Liability

10.1 Save where Goods manufactured by Surtex Instruments are held to be defective as defined in Part 1 of the Consumer Protection Act 1987, Surtex Instruments sole obligation in the event of any missing or defective Goods, shall be to repair or replace the Goods.

10.2 Surtex Instruments shall not be liable in respect of consequential loss, loss of profits, damage to the property, loss of goodwill, loss of business opportunity, wasted expenditure, cost of mitigation arising out of or occasioned by any fault or defect in the Goods supplied or any other losses howsoever caused.

10.3 The maximum total liability under or arising out of in connection with this Agreement will not exceed the total of the Contract value.

10.4 Nothing in this Agreement shall exclude or limit either party's liability for death or personal injury resulting from negligence or their fraudulent acts, omissions or statements or for infringement of third party's intellectual property rights.

10.5 For the purpose of the Health and Safety at Work Act 1974, Surtex Instruments relies upon the testing examination and research carried out by the suppliers to it of propriety equipment and component parts of Goods.

10.6 This clause 10 shall survive the termination of the contract.

11. Return of Goods

11.1 In cases where Goods are not defective and the customer requests to return the Goods, Surtex Instruments shall be under no contractual obligation to accept the return except in the event of any error on its parts as to the amount or type of Goods delivered.

- 11.2 Any requests to return must be made to Surtex Customer Support Centre within ten working days of the date of actual delivery.
- 11.3 The return of Goods to correct an error in delivery or ordering will only be considered if the Customer Care Team is notified immediately or in any event within 48 hours of delivery to the Customer. Goods must be returned to Surtex Instruments within 5 days of delivery to the customer to correct an error in delivery or ordering.
- 11.4 For the avoidance of doubt, unless defective, the returns of Goods as detailed in sections 11.2, 11.4, 11.5 and 11.6 must be unused, undamaged and in the original packaging. The Goods must be the same batch as originally supplied by Surtex Instruments and are not falsified/counterfeit. All goods are individually assessed by Surtex Instruments before being authorised to return.
- 11.5 Return of Goods for any reason shall require prior consent from Surtex Instruments which shall be sent solely at the discretion of Surtex Instruments. To obtain consent, the Customer Care Team must be notified. Consideration to requests for a return may be given if:
- a) of a bona fide nature;
 - b) made within 10 working days of the actual delivery; and
 - c) unless defective, the Goods must be unused, undamaged and in the original undamaged packaging. The Goods must be the same batch as originally supplied by Surtex Instruments and not falsified/counterfeit.
- 11.6 On the customer contacting Surtex Instruments to request a return, the Customer will be issued with a returns merchandise authorisation number by Surtex Instruments. Goods returned without the prior written approval of Surtex Instruments may be returned to the customer or disposed of at the absolute discretion of the company.
- 11.7 Goods returned will be subjected to the following charges:
- a) for palletised items there will be a standard charge of £75.00 per pallet for any return uplifted by Surtex Instruments.
 - b) for returns of small parcel there will be a minimum £15.00 charge per parcel and a 30% re-stocking charge.
 - c) the event of return resulting from an error on the part of Surtex Instruments in relation to the amount or type of Goods delivered, no charges under this clause 11.7 will apply.
- 11.8 In the event, that any Goods are subject to be called by Surtex Instruments for the purpose of recall, the customer shall provide to Surtex Instruments as much information as it is reasonably possible regarding the whereabouts of the Goods.

12. Cancellation Policy

- 12.1 In the event of cancellation before delivery and if returned after delivery where products are not defective, there will be a re-stocking charge of not less than 30% of the invoice value charged by Surtex Instruments.
- 12.2 Cancellation of an order will only be agreed by Surtex Instruments at its sole discretion, on condition that all costs and expenses incurred by Surtex Instruments up to the time of cancellation and loss of profits and other loss or damage resulting to Surtex Instruments of such cancellation will be reimbursed by the Customer to Surtex Instruments forthwith.

13. Specifications

Surtex Instruments reserve the right to alter or change the specification and dimension of the Goods supplied with reasonable limits having regard to the nature of the Goods. These do not materially affect the quality or fitness for purpose of Goods. Dimensions specified by Surtex Instruments are to be treated as an approximate only unless the Customer specifically states in writing that exact dimensions are required. Our website and catalogues display the product images as accurately as possible. However, Surtex Instruments cannot guarantee the finish/colour you see matches the actual product as the display of the finish and or colour depends in part, upon your monitor and its settings.

14. Marking and Instructions

- 14.1 No name, mark, numbering, colouring, appearance or log on the goods will be obscured, removed or concealed by the Customer.
- 14.2 The Customer will not repackage or alter the presentation of Goods and it will not assist, cause, or enable any other party to do any of the said acts or deal in Goods or packaging which have been subject to such acts.
- 14.3 The Customer acknowledges that it is under a duty to pass on to its customers (where appropriate) all instructions, information and warnings supplied by Surtex Instruments with the Goods.

15. Confidential Information

- 15.1 A party shall treat the Contract as private and confidential and neither party shall publish or disclose any particulars without the prior written consent of the other with the exceptions of 15.2 below.
- 15.2 The obligations expressed in 15.1 above shall not apply to any information which:
- a) Is or subsequently comes into the public domain other than by breach of this clause;
 - b) The disclosure of which is required to be disclosed by law, any governmental or regulatory authority or by a court of competent jurisdiction;
 - c) Comes into the possession of one of the parties prior to its disclosure by the other, or which is acquired lawfully and in good faith from an independent third party.
- 15.3 On the conclusion or termination of the Contract, both parties shall destroy all copies of confidential information obtained from the other and the obligation relating to the confidentiality shall continue for a period of 10 years.
- 15.4 The Customer shall not, without the prior written consent of Surtex Instruments, advertise or make known to any third that Surtex Instruments provided Goods to the Customer.

16. Insolvency

- 16.1 Without limiting its other rights or remedies, Surtex Instruments shall be entitled to cancel the contract, in whole or in part, by notice in writing if:
- a) The Customer makes a voluntary arrangement with its creditors or (being an individual firm) becomes bankrupt or (being a company) becomes subject to an administration order or goes into liquidation (otherwise than for purpose of amalgamation or reconstruction);
 - b) An encumbrancer takes possession, or a receiver is appointed, of any of the property or assets of the Customer.
 - c) The Customer ceases, or threatens to cease, to carry on business; d) Surtex Instruments reasonably apprehends that any of the events mentioned above is about to occur in relation to the Customer and notifies the Customer accordingly.

17. Sub-Contractors

- 17.1 Surtex Instruments may assign the Contractor any part of it to any company, firm or organization.
- 17.2 The Customer shall not be entitled to assign the Contractor any part of it without the prior written consent of Surtex Instruments (such consent not to be unreasonably withheld or delayed).

18. Force Majeure

- 18.1 Surtex Instruments shall not be responsible for any failure to fulfil its obligations under these conditions and/or in relation to the Goods if such failure is caused by an event which is beyond its reasonable control including acts of God, war, armed conflict, acts of terrorism, riot, strikes, industrial action (including action involving Surtex Instruments employees), fire, flood, any natural disaster, any defaults by Surtex Instruments suppliers or subcontractors, difficulties obtaining workmen or materials, and breakdown of machinery.
- 18.2 If such event continues for more than one month, Surtex Instruments may terminate the Contract without liability.

19. Waiver

19.1 waiver of any right or remedy under the contract or law is only effective if given in writing and shall not be deemed a waiver of any subsequent breach or default. No failure or delay by a party to exercise any right or remedy provided under the Contract or by law shall constitute a waiver of that or any other right or remedy. No single or partial exercise of such right or remedy shall prevent or restrict the further exercise of that or any other right or remedy.

20. Severance

20.1 any provision or part-provision of the Contract is or becomes invalid, illegal or unenforceable, it shall be deemed modified to the minimum extent necessary to make it valid, legal and enforceable whilst retaining the risk and reward between the parties. If such modification is not possible, the relevant provision or part-provision under this clause shall not affect the validity and enforceability of the rest of the Contract.

21. Variation

21.1 as set out in these Conditions, no variation of the Contract, including the introduction for any additional terms and conditions, shall become effective unless it is agreed in writing and signed by Surtex Instruments.

22. General

22.1 rights and remedies of Surtex Instruments set out in these conditions shall be in additions and without prejudice to any other rights and remedies which may be available to Surtex Instruments at common law or under the statute.

23. Governing Law and Jurisdiction

23.1 The contract and any dispute or claim arising out of or in connection with it or its subject matter or formation (including not-contractual disputes or claims) shall be governed by and construed in accordance with the law of England and Wales.

23.2 Each party irrevocably agrees that the courts of England and Wales shall have exclusive jurisdiction to settle any dispute or claim arising out of or in connection with his agreement or its subject matter or formation (including non-contractual disputes or claims).

23.3 The schedules to the Uniform Law of International Sales Act 1967 shall not in any circumstances apply to the contract.

24. Entire Agreement

24.1 This contract constitutes the whole agreement and understanding between the parties in relation to its subject matter and supersedes any previous arrangement, understanding, representations, (including any information or data set out in any sales and marketing literature), or agreement between them relating to the subject matter of this Agreement.

24.2 Each party acknowledges that, in entering into this Agreement, it has not relied on any statement, assurance or warranty (whether made negligently or innocently) other than those expressly set out in this Agreement and has no rights and remedies in respect thereof.

25. Third-Party Rights

25.1 term of this agreement shall be enforceable under the Contracts (Rights of Third Parties) Act 1999 by any legal entity who is not a party to this Agreement.

26. Notices

26.1 communications between the parties about the Contract shall be in writing and delivered by pre-paid first-class post or by hand to the party's registered office, principal place of business or such other address as may at the relevant time have been notified pursuant to this provision to the party giving notice. In the absence of evidence of earlier receipt, any notices shall be deemed to be duly served:

- a) If sent by first class post, two working days after posting; or
- b) If delivered personally, when left at the relevant address.



COPYRIGHT NOTICE

The copyright, trademarks, domain names and other intellectual property rights in all materials and information in this presentation belongs to Surtex Instruments Ltd. All rights are reserved. Technical alterations are possible. This presentation may be used for no other purpose than offering, buying and selling of Surtex Instruments products. No part may be reproduced or copied in any form. In the event of misuse we retain the right to recall our catalogues and take appropriate legal action.

DISCLAIMER

This documents provides general information about Surtex Instruments Ltd, its products and services, and summarises general capabilities and offerings, which we deem to be relevant to our customers. Whilst Surtex Instruments has taken appropriate steps to ensure the accuracy of the information contained in the document Surtex Instruments gives no warranty regarding the accuracy or completeness of such information.

The presentation was prepared to provide information and does not constitute a contract. Surtex reserves the right, without prior notice, to change, delete, supplement, or otherwise amend at any time the information, images and offerings contained in the presentation or other documents. Surtex shall not be liable for any loss or damage of whatever nature (whether direct, indirect, consequential or other) may arise as a result of any third party relying on the information contained in this document.

For further detailed information, prices, terms and conditions, customer should contact Surtex Instruments at sales@surtex-instruments.co.uk.

© 2021 **SURTEX INSTRUMENTS**. ALL RIGHTS RESERVED. PRINTED IN UNITED KINGDOM. BT1-01 Rev 1.0



Unit 202 Kingspark Business Centre
152-178 Kingston Road, New Malden
Surrey KT3 3ST United Kingdom
Phone: +44 (0) 208 123 3513

E-mail: sales@surtex-instruments.co.uk
Website: www.surtex-instruments.co.uk



A member of the ABHI

